

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES

Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- ✓ TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**

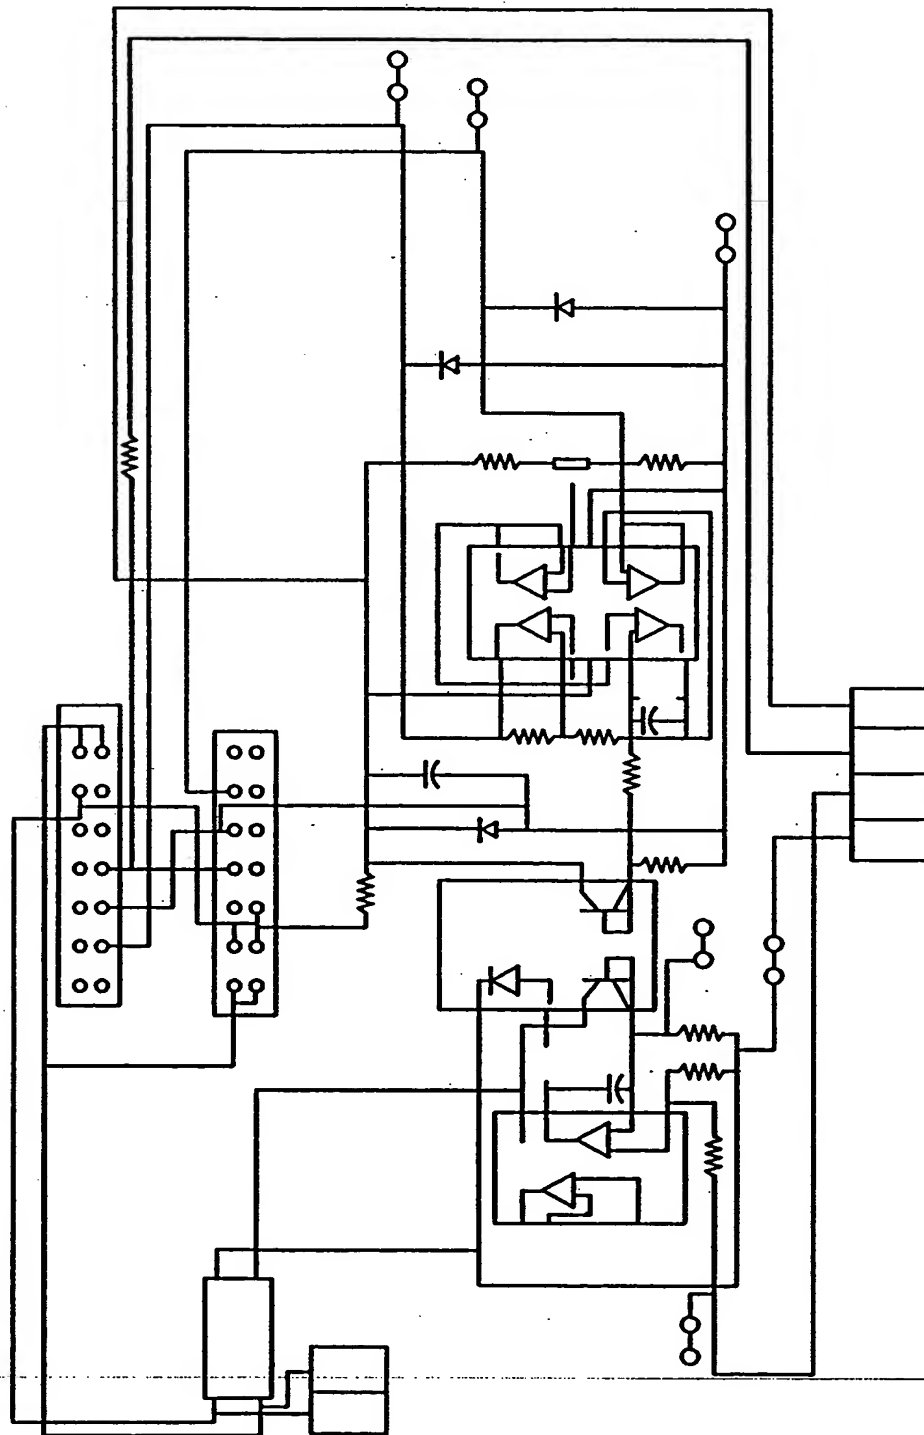


Fig. 1

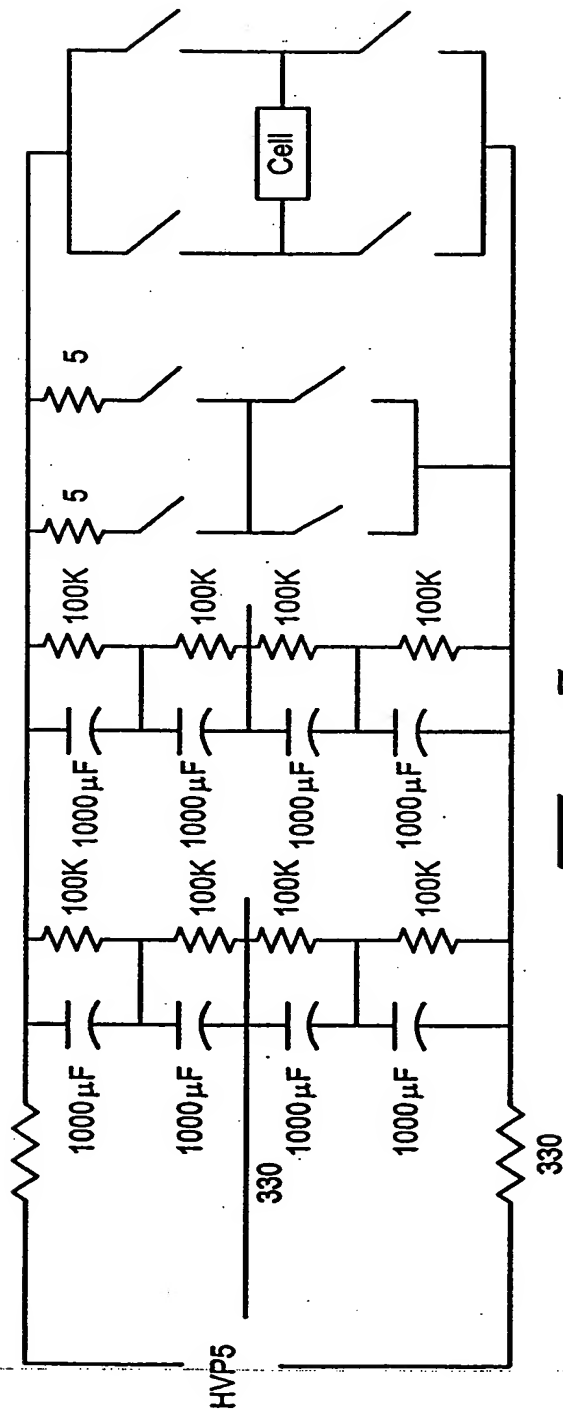


Fig. 2

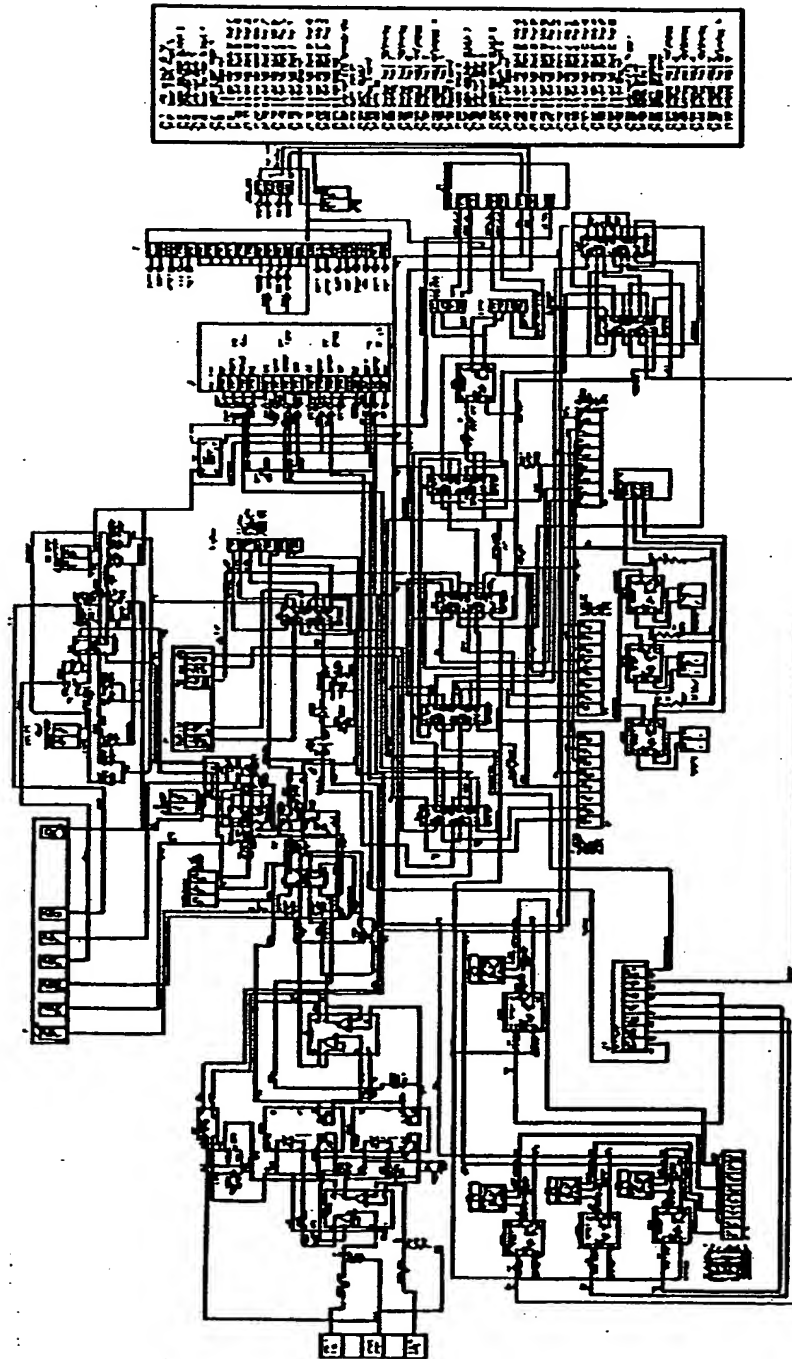


Fig. 3

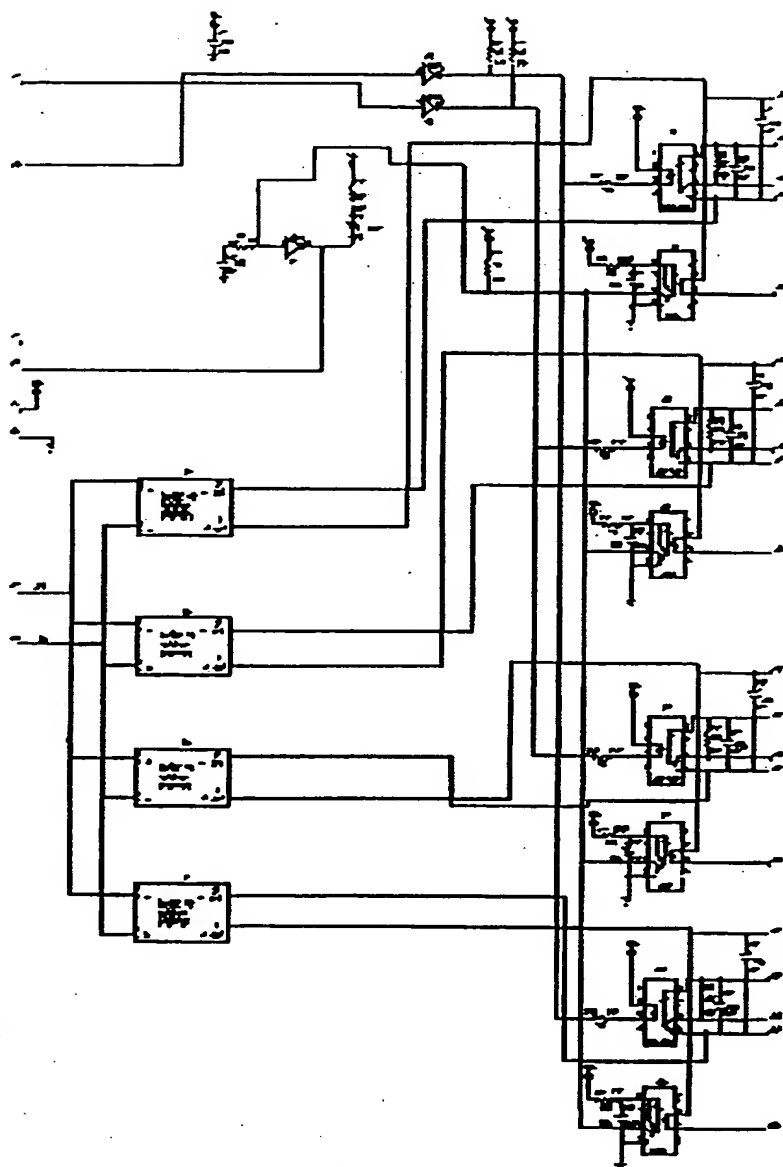


Fig. 4

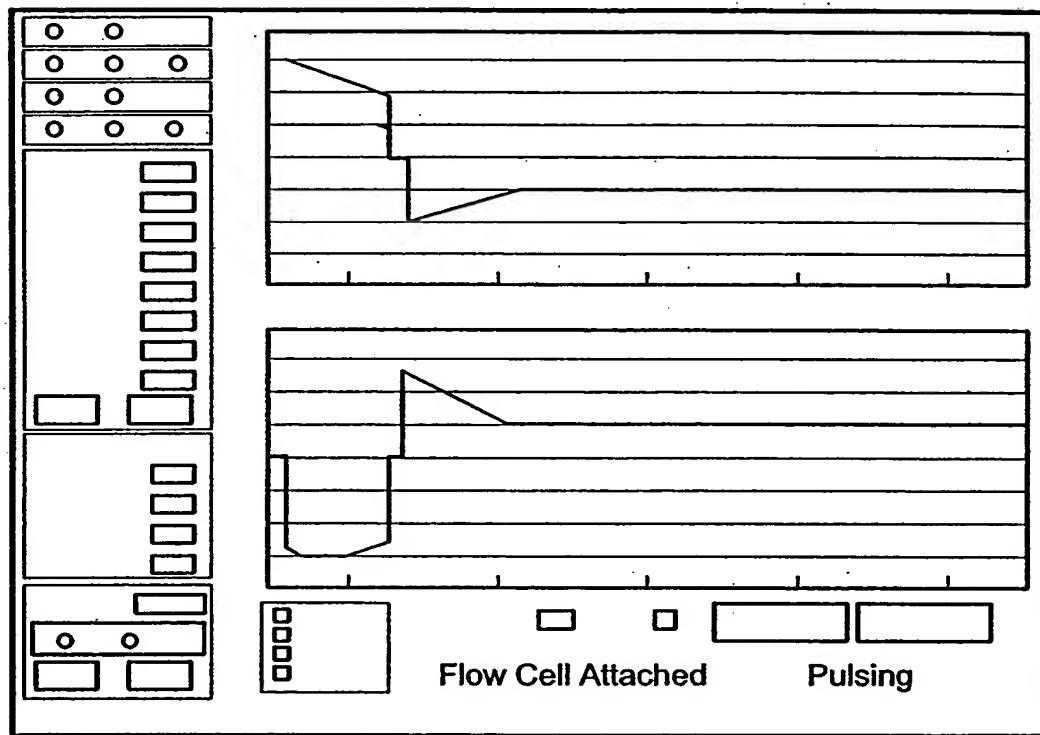


Fig. 5

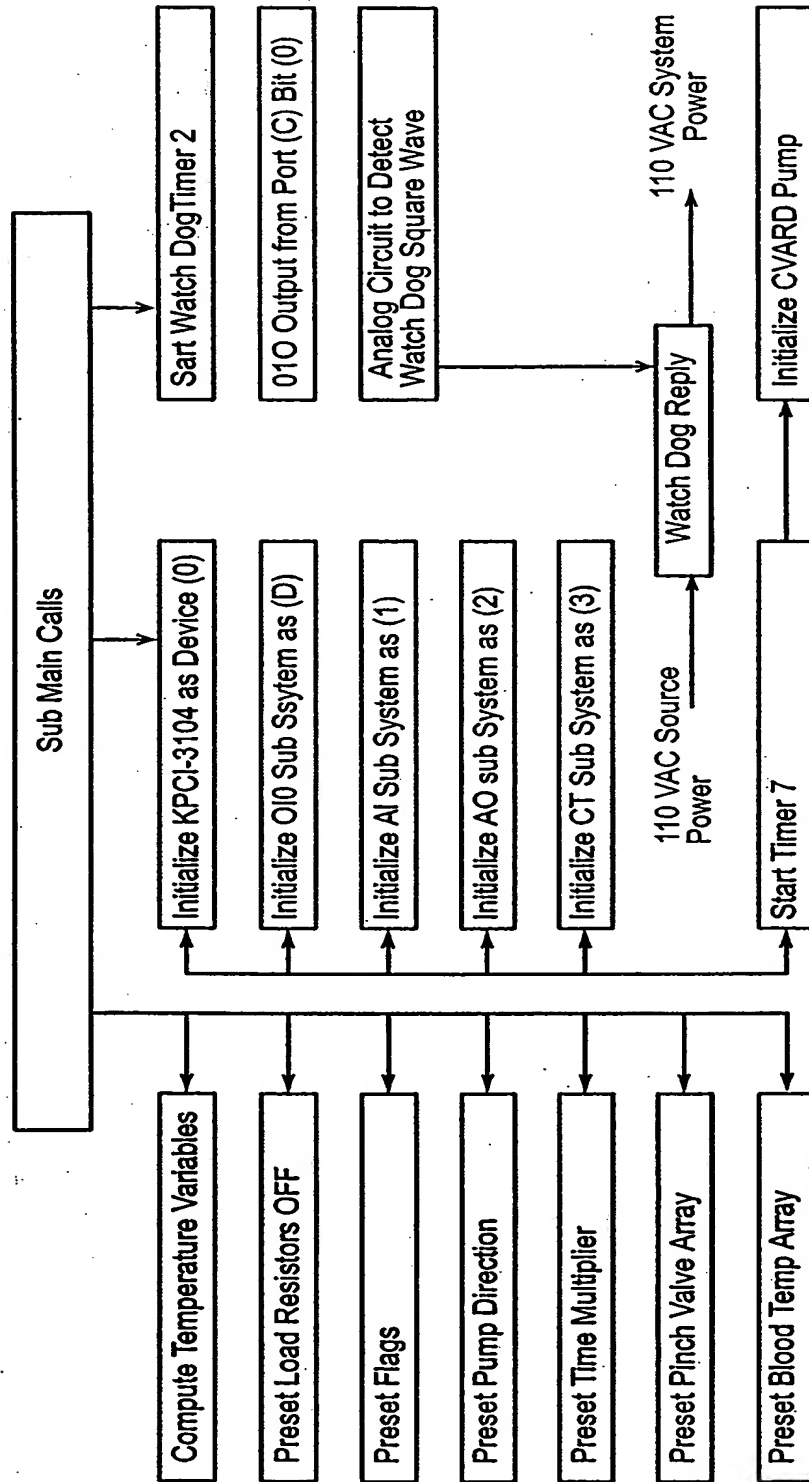


Fig. 6

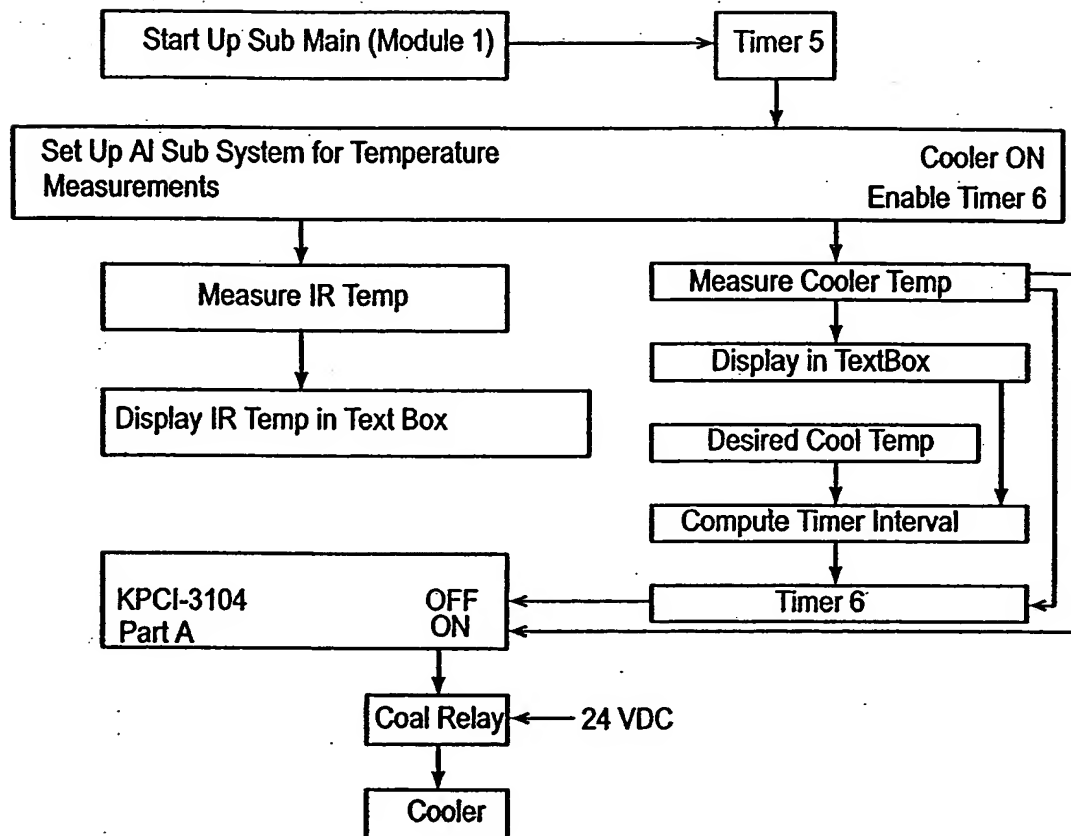


Fig. 1

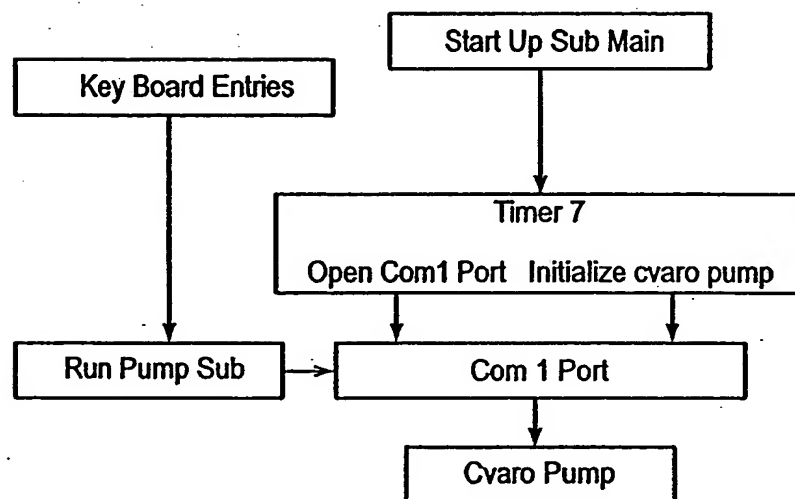


Fig. 8

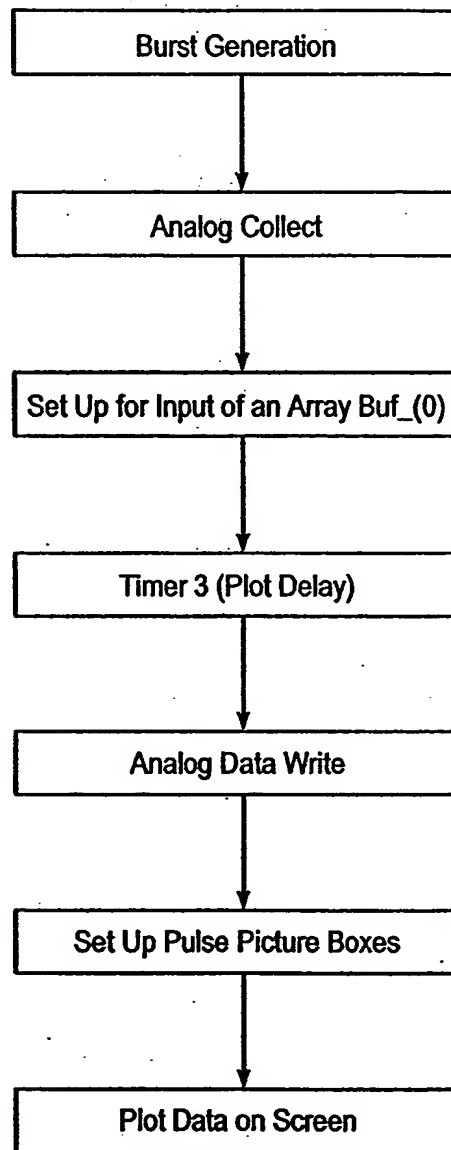


Fig. 9

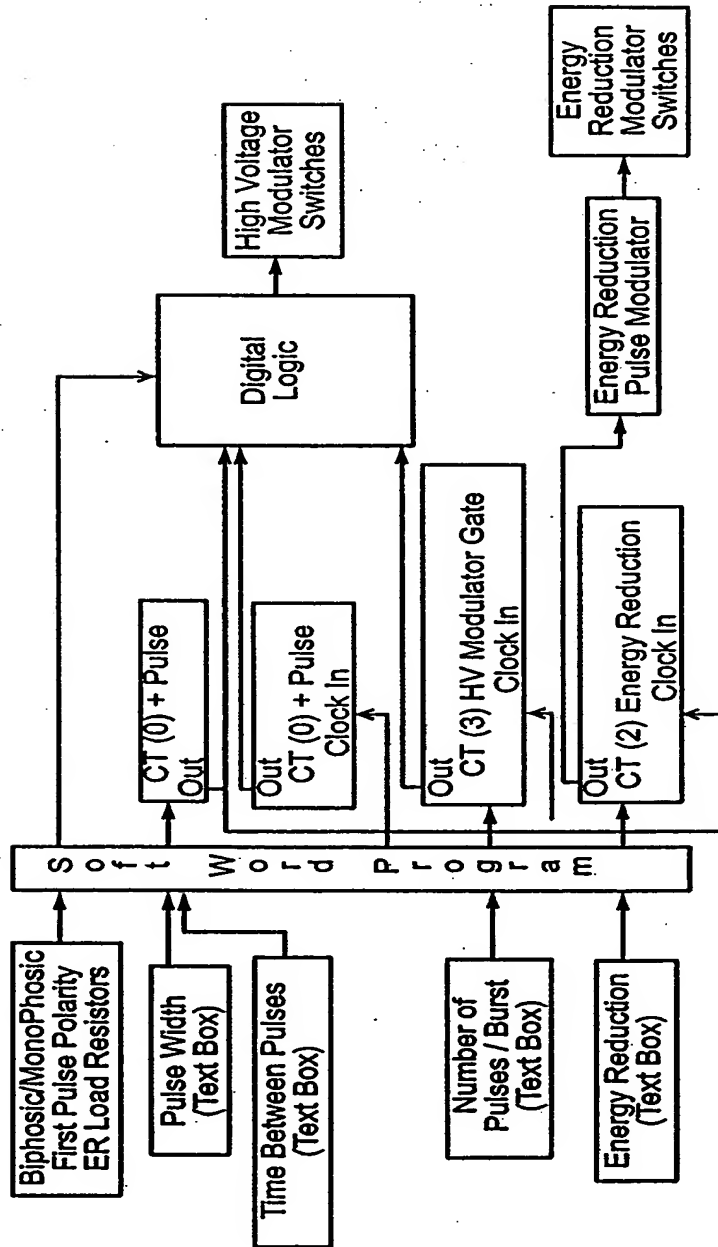


Fig. III

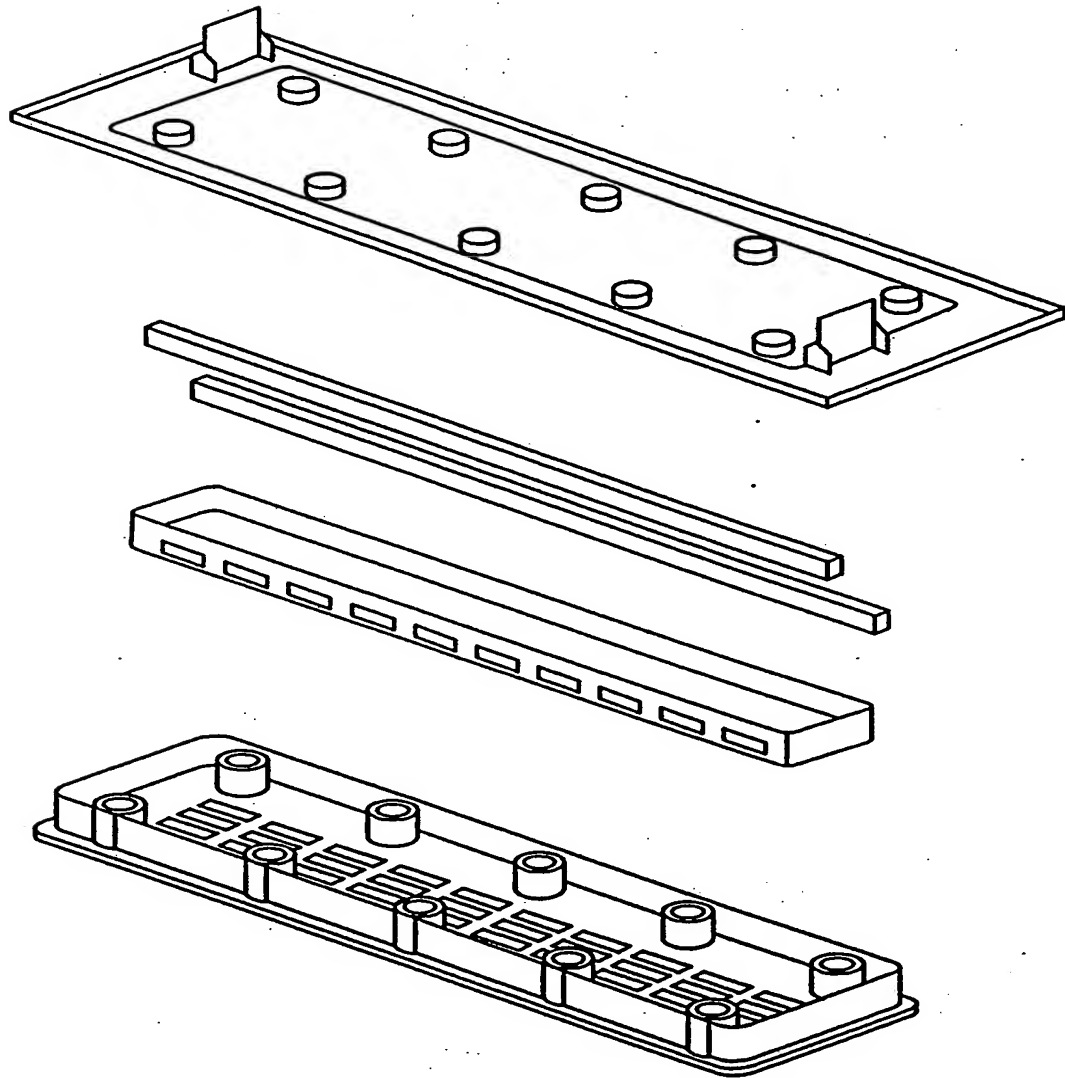


Fig. 11

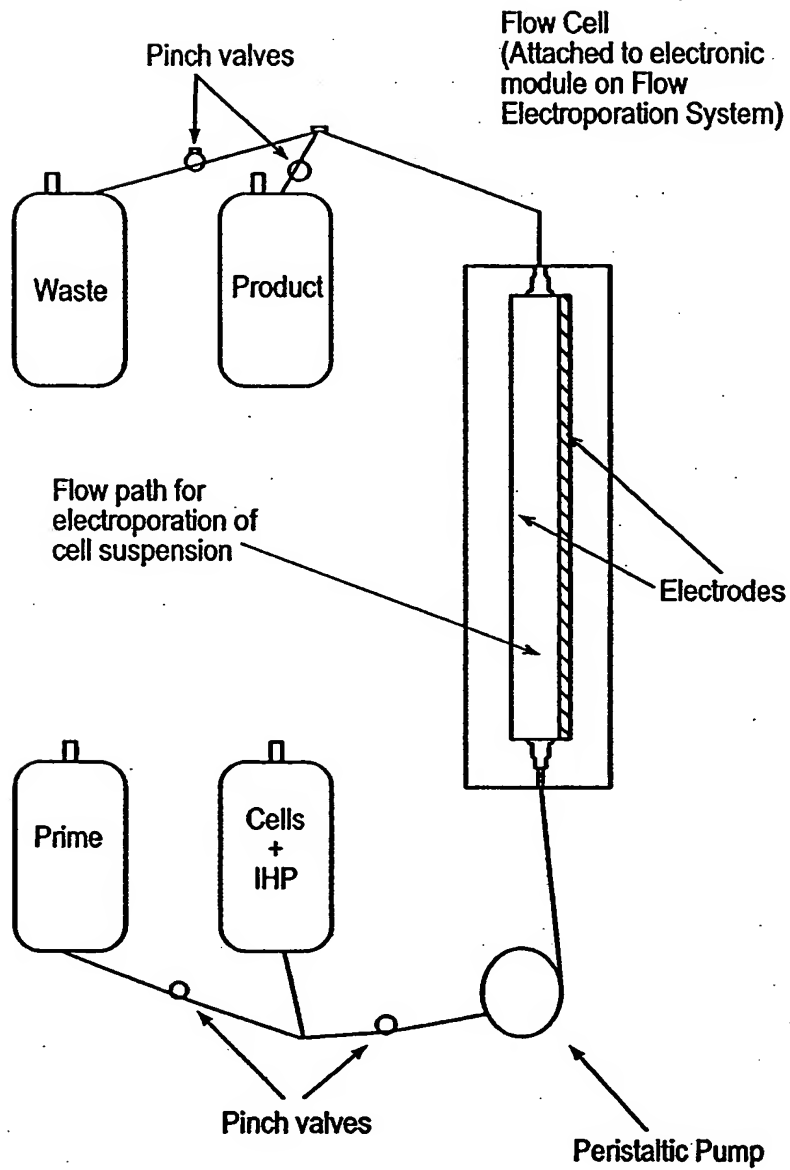
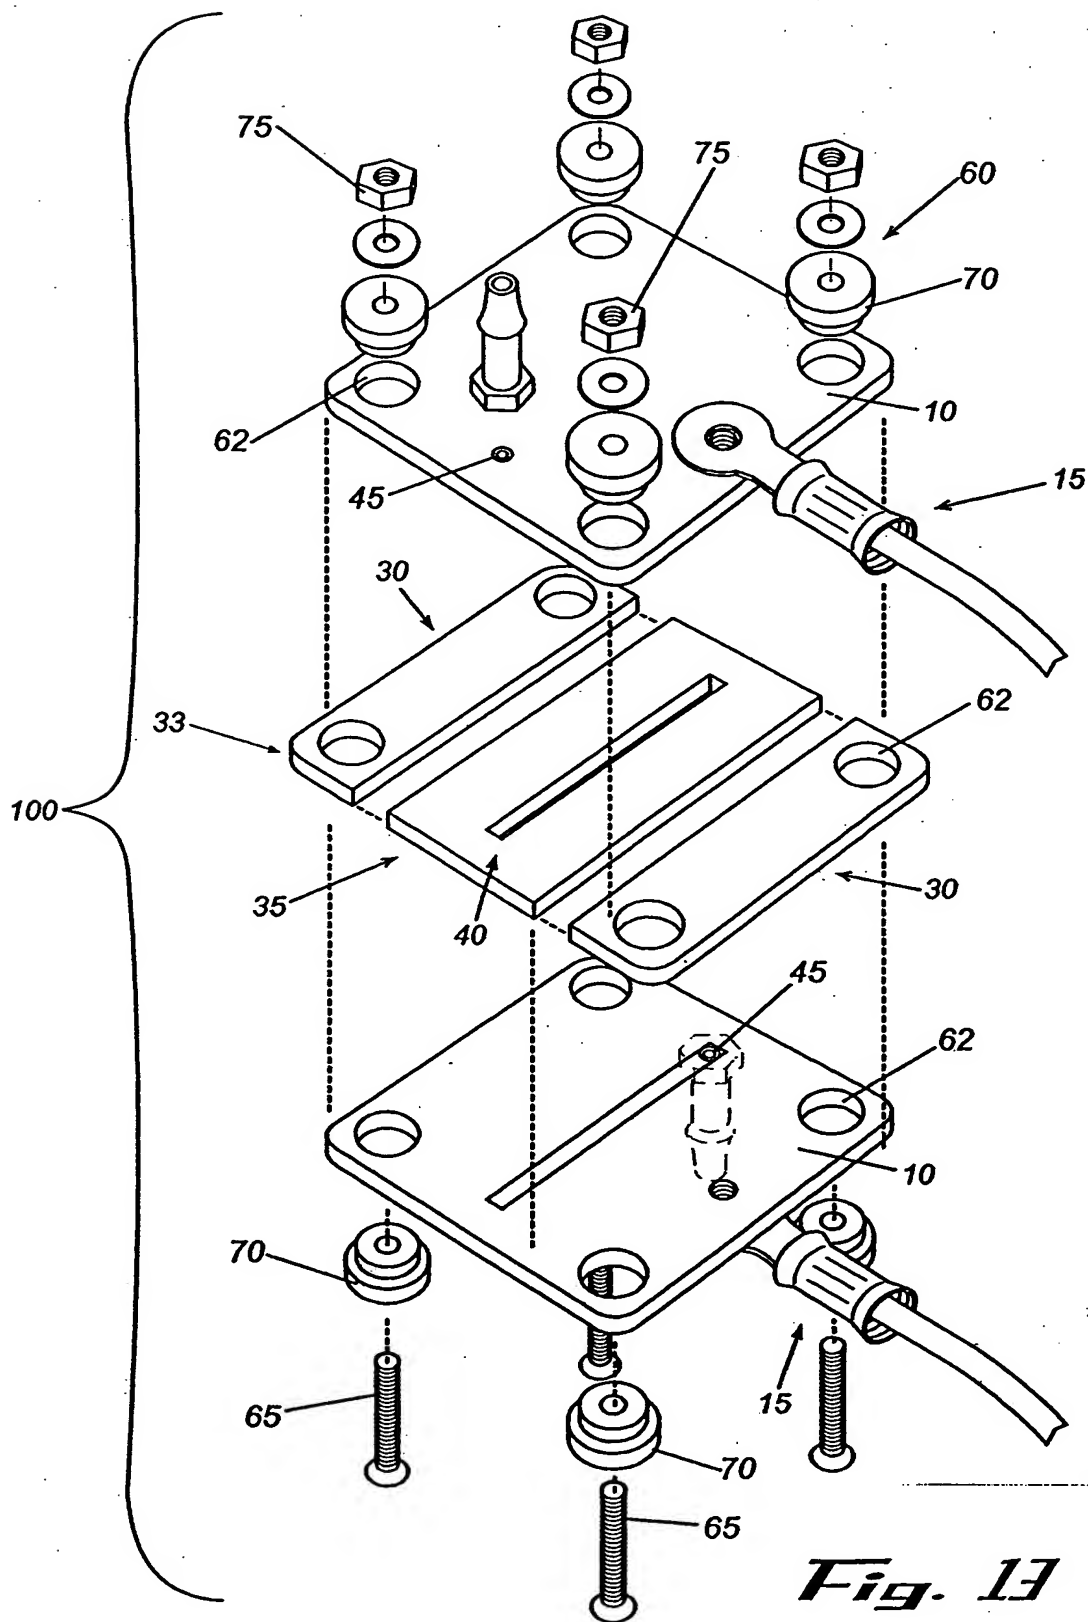


Fig. 12



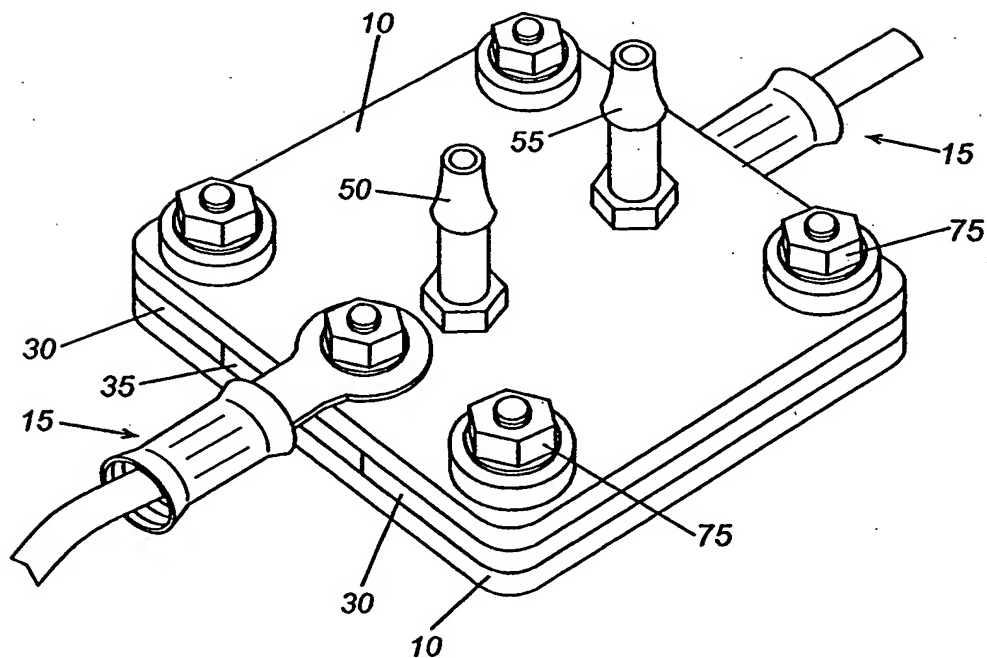


Fig. 14

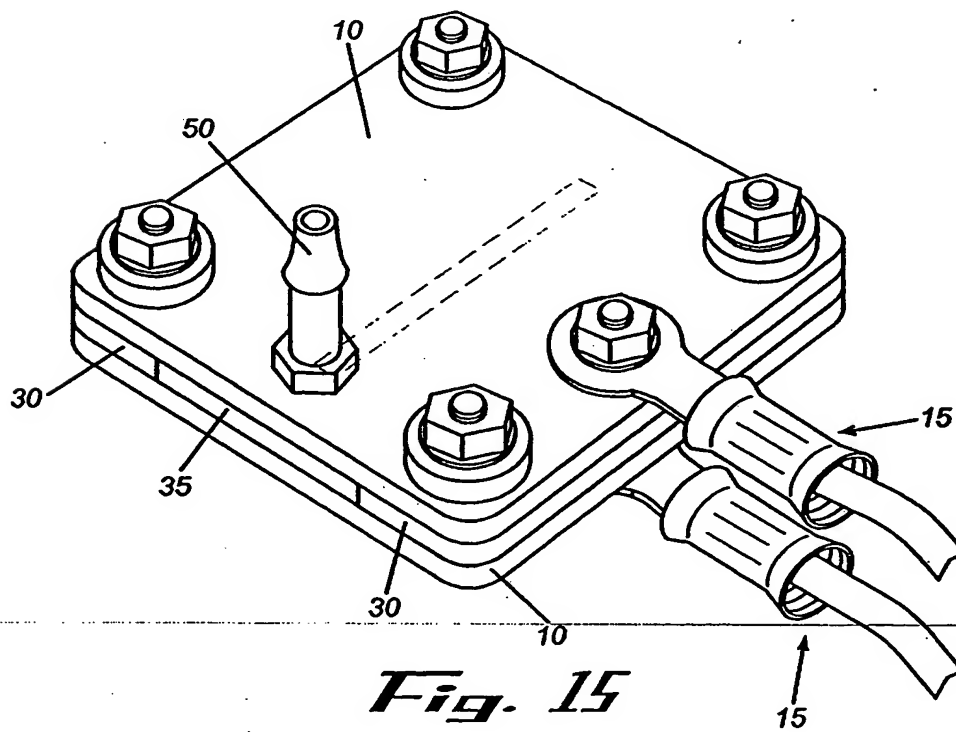


Fig. 15



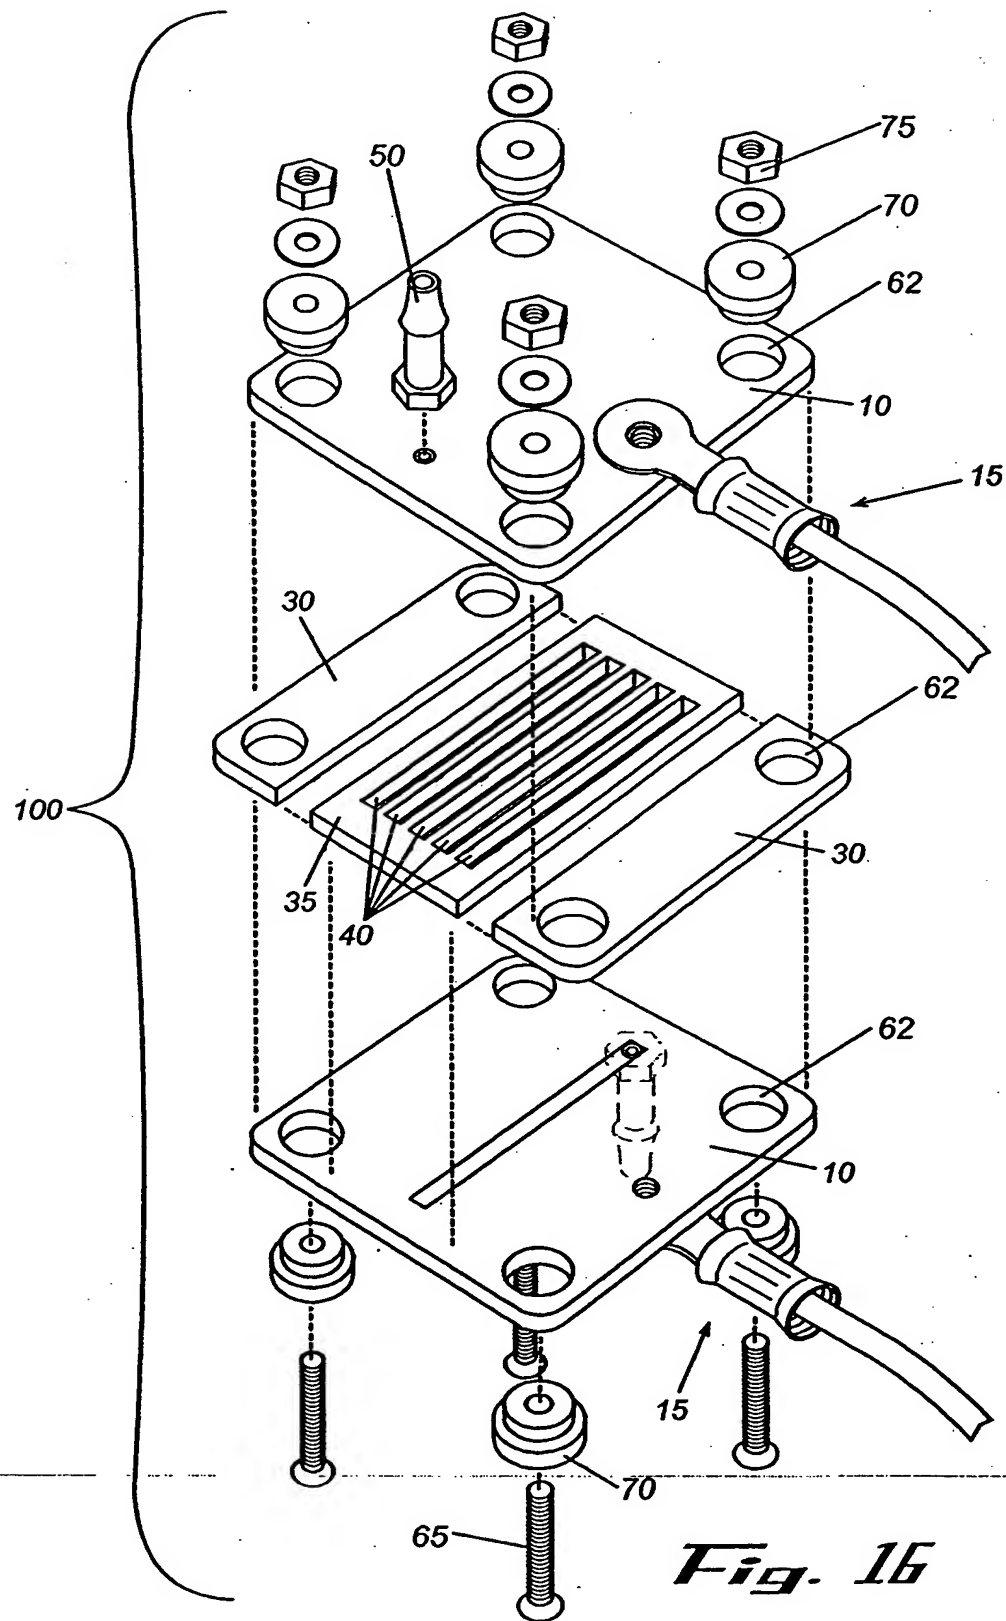


Fig. 16



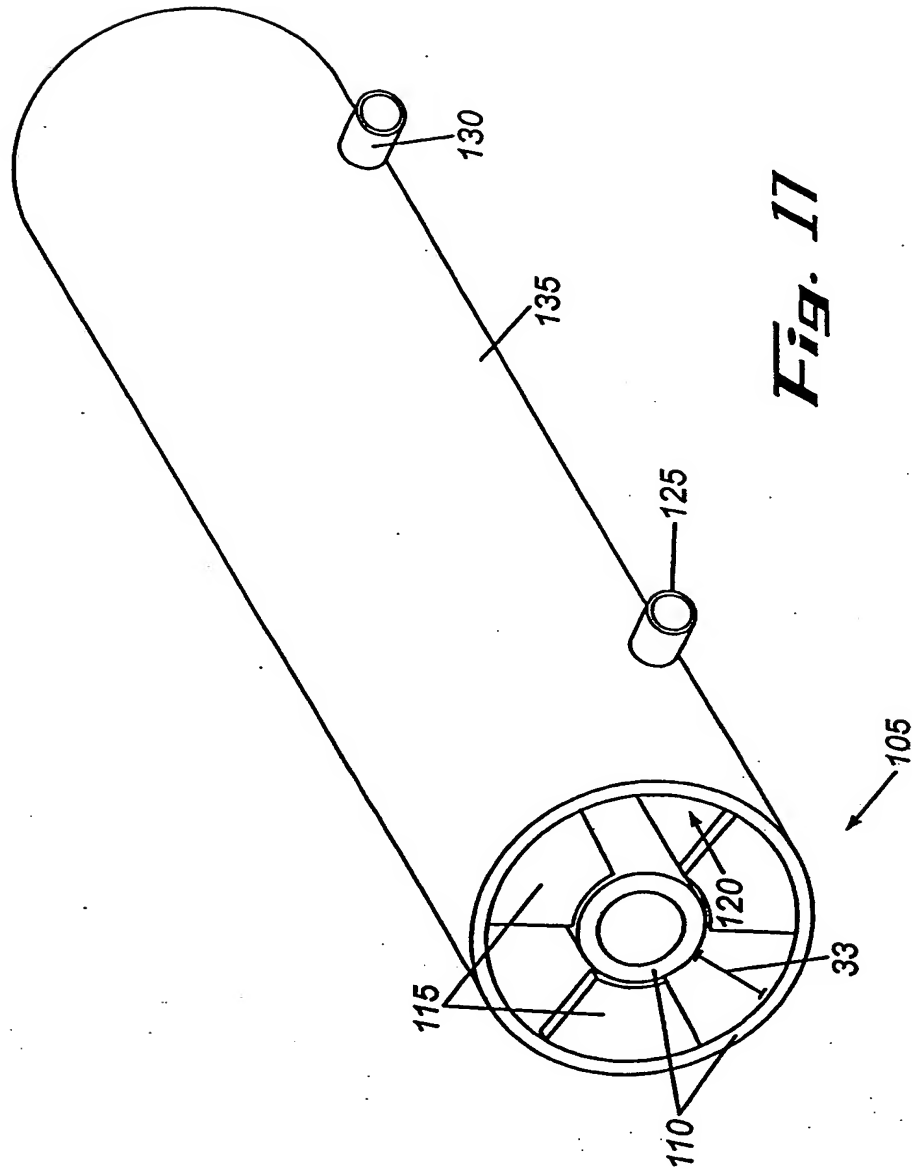

Consistency of RBC product performance with numerous donors

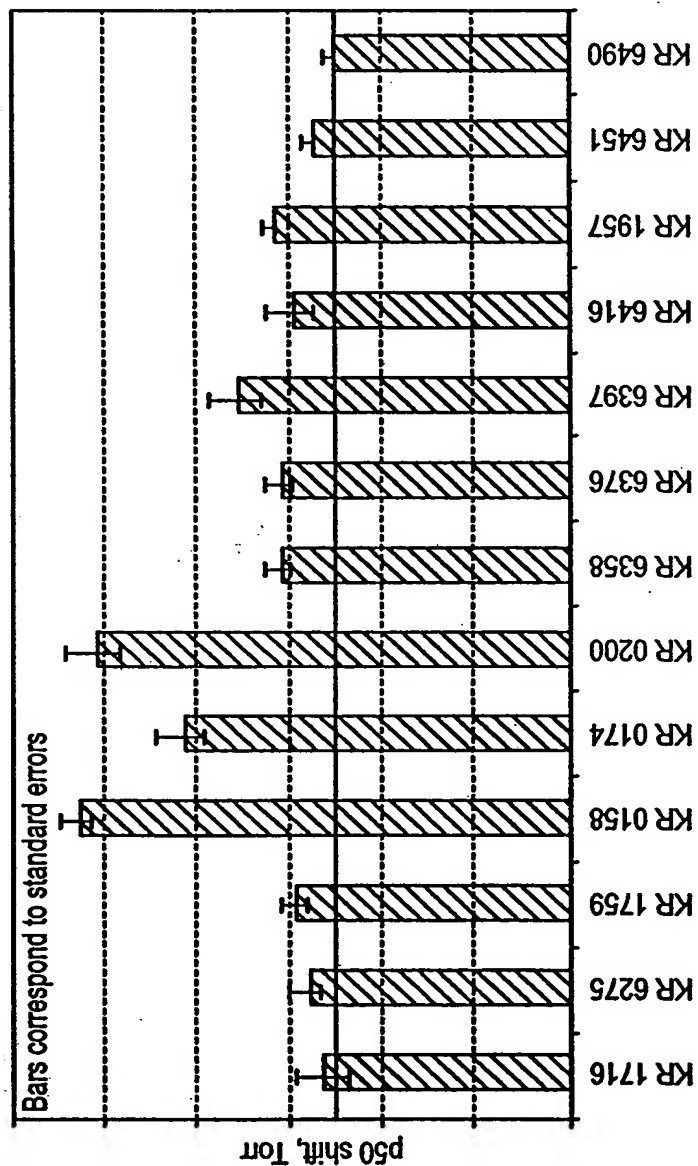

Donor ID
Fig. 1A

Large Volume Transfected Fibroblasts Are Viable
and Express Functional Transgene in vivo

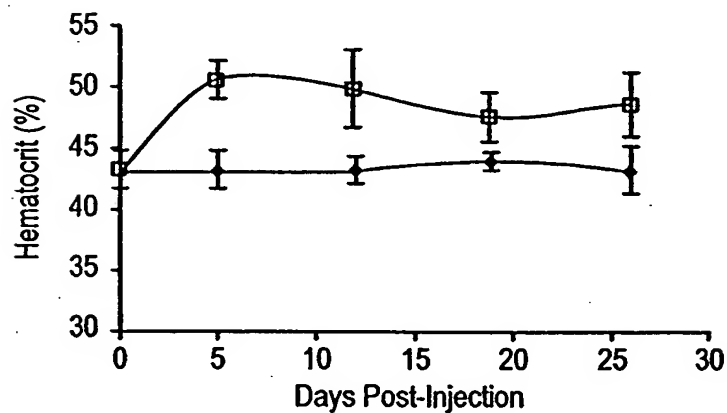


Fig. 19

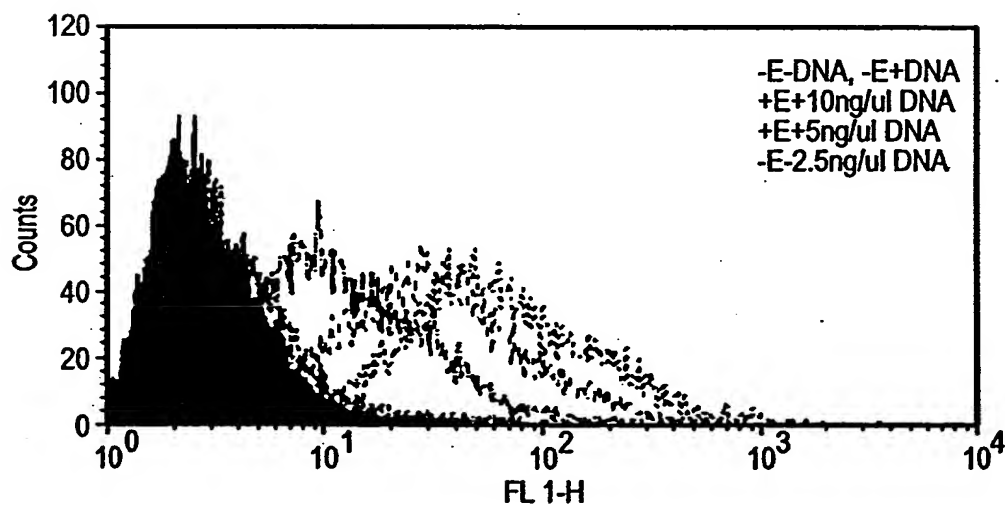


Fig. 20

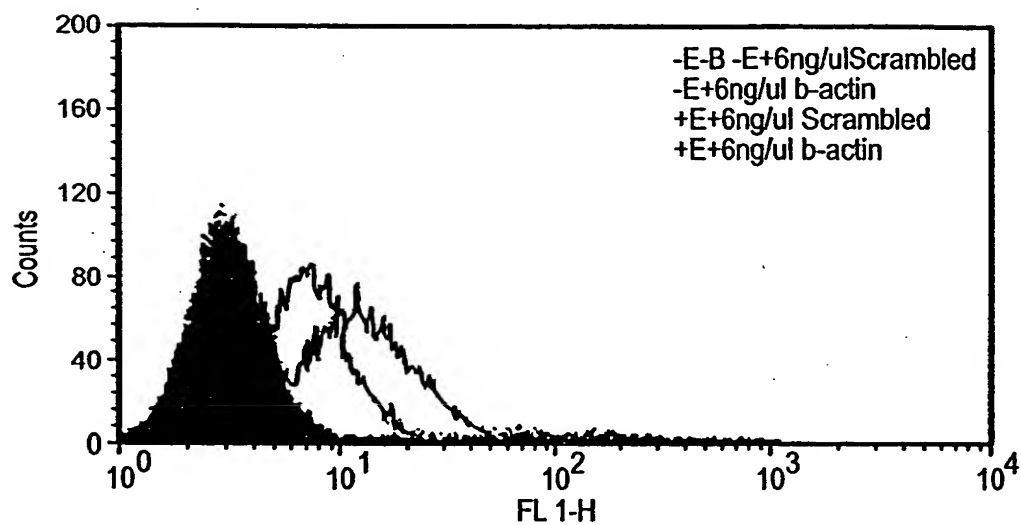


Fig. 21

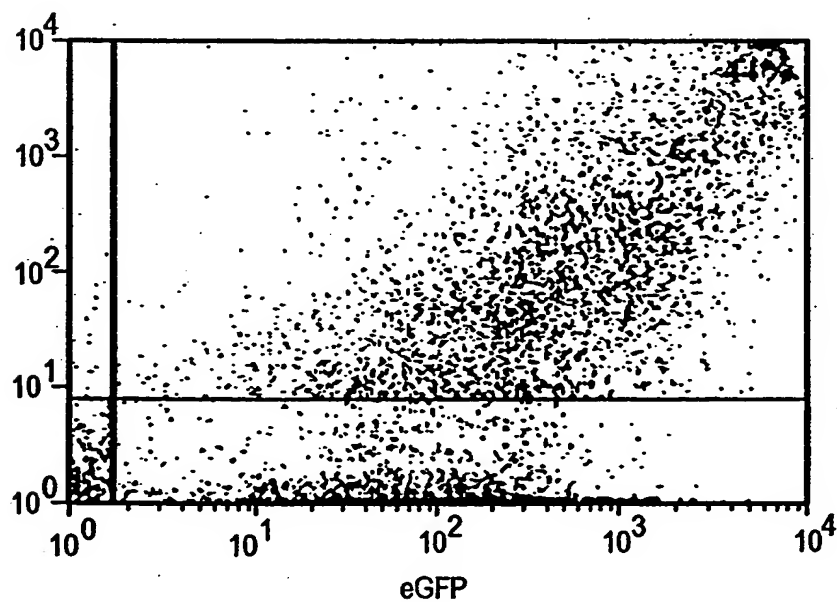


Fig. 22

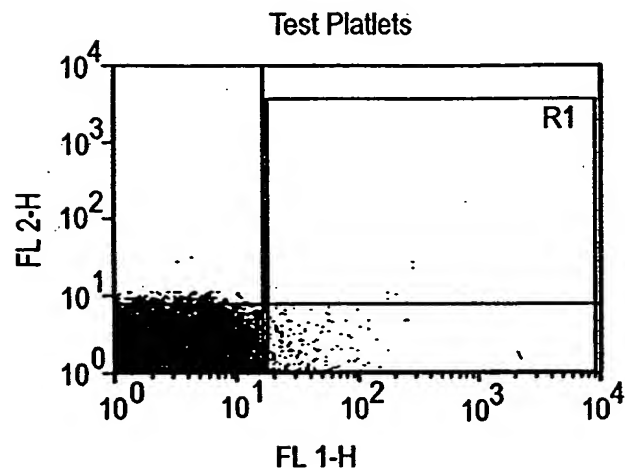


Fig. 23A

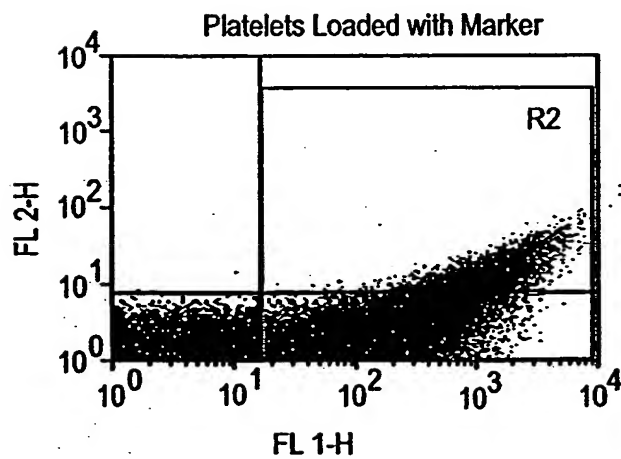


Fig. 23B

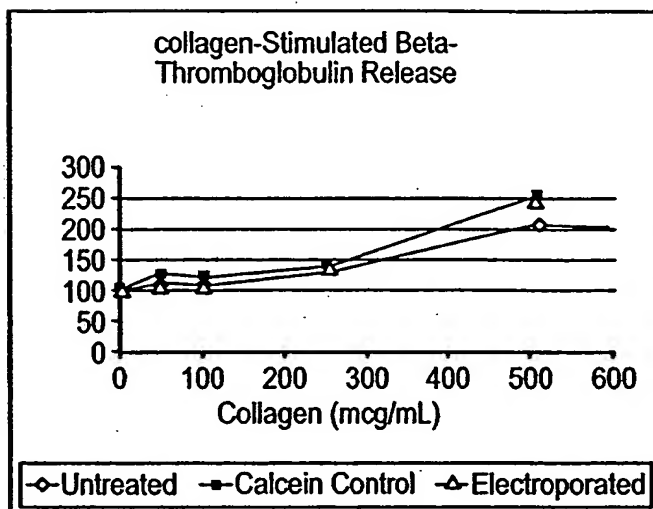


Fig. 24A

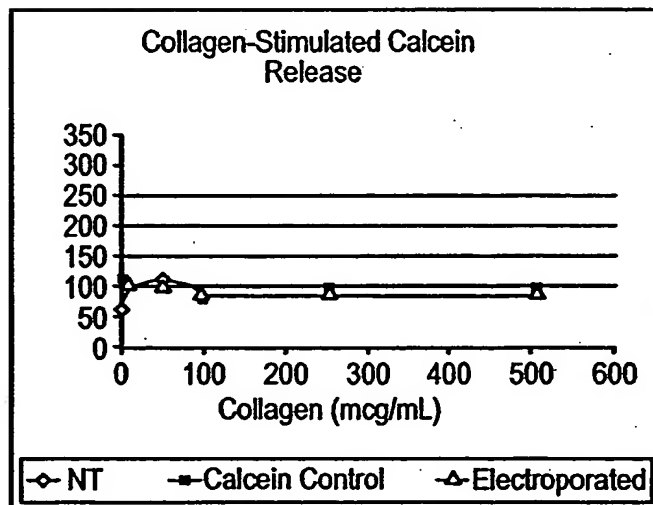


Fig. 24B

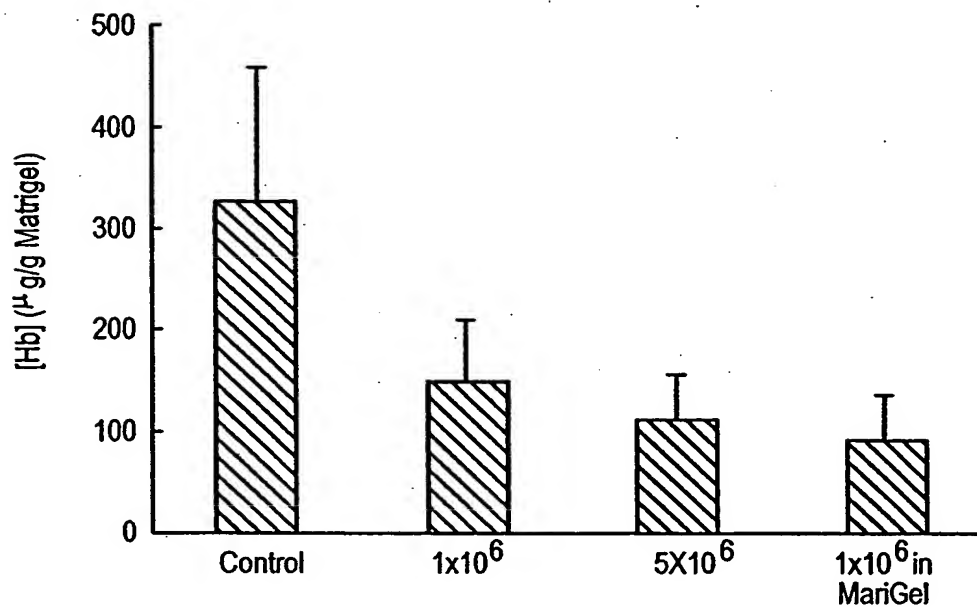


Fig. 25

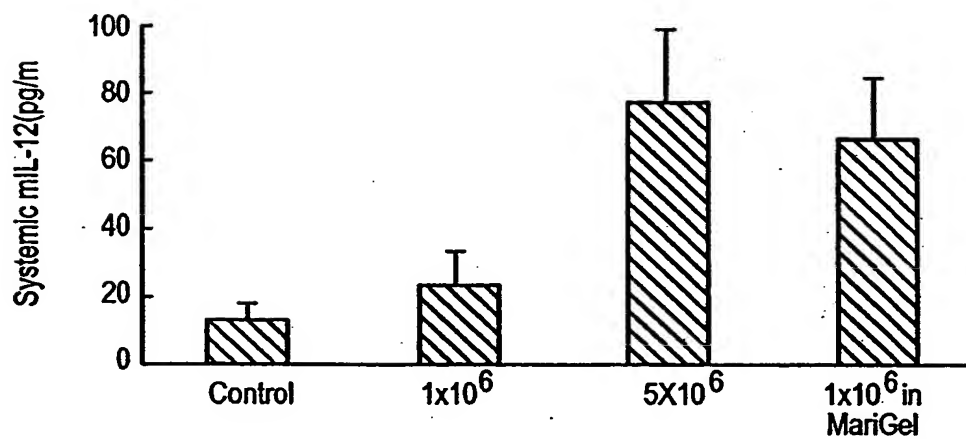


Fig. 26

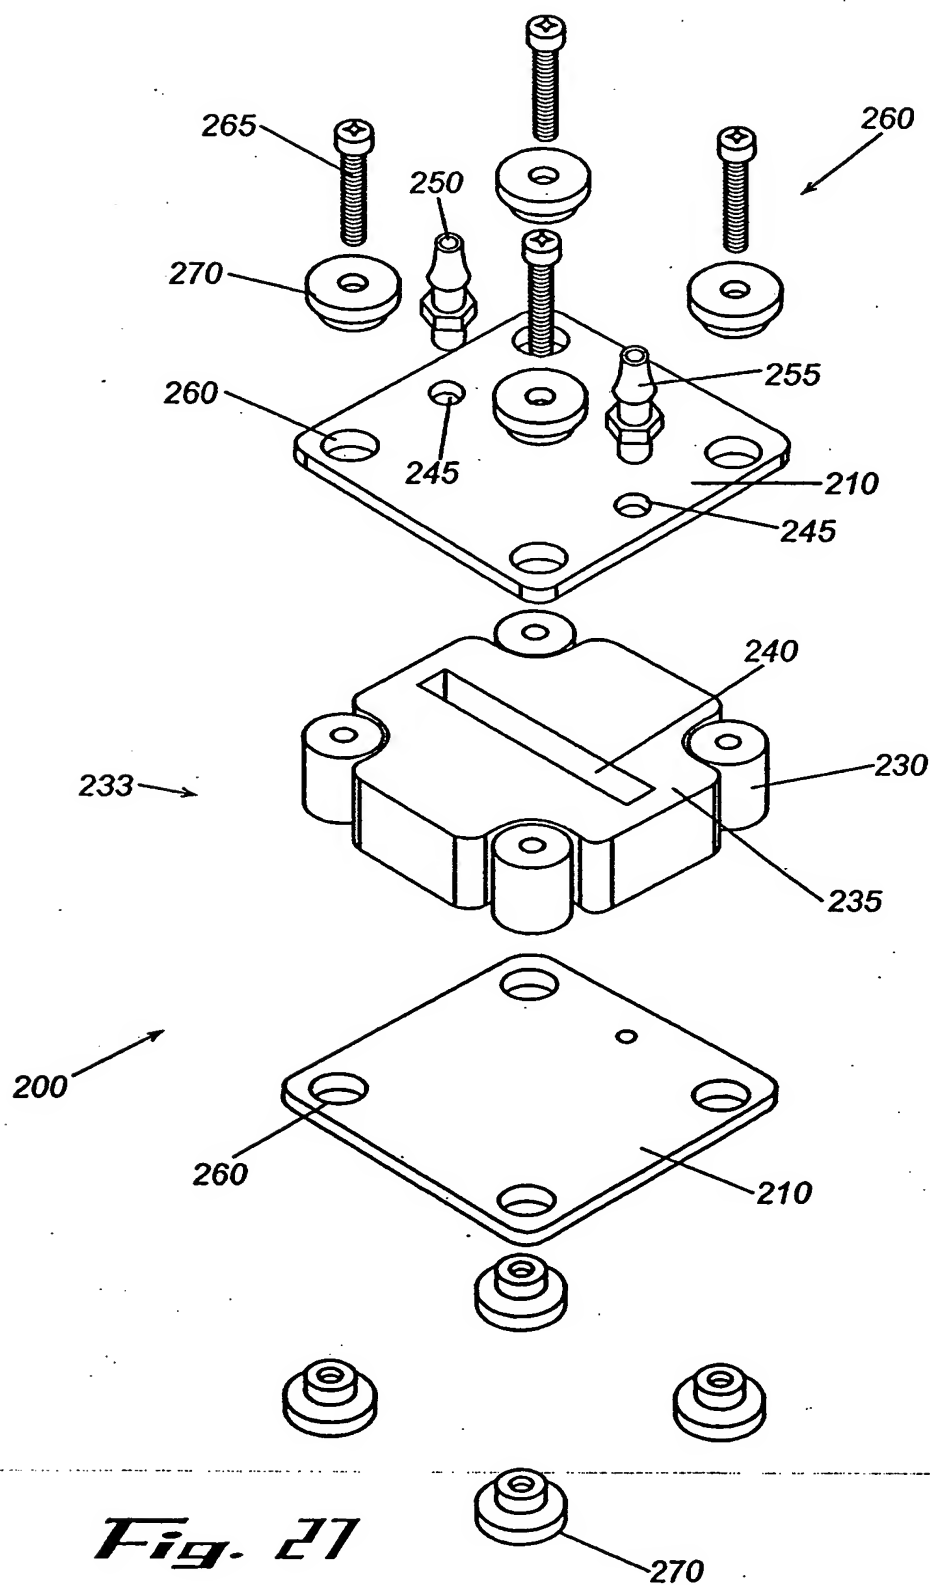


Fig. 21

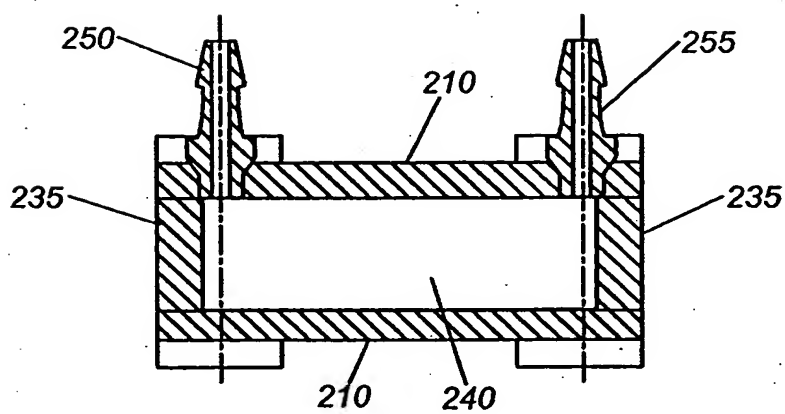


Fig. 28

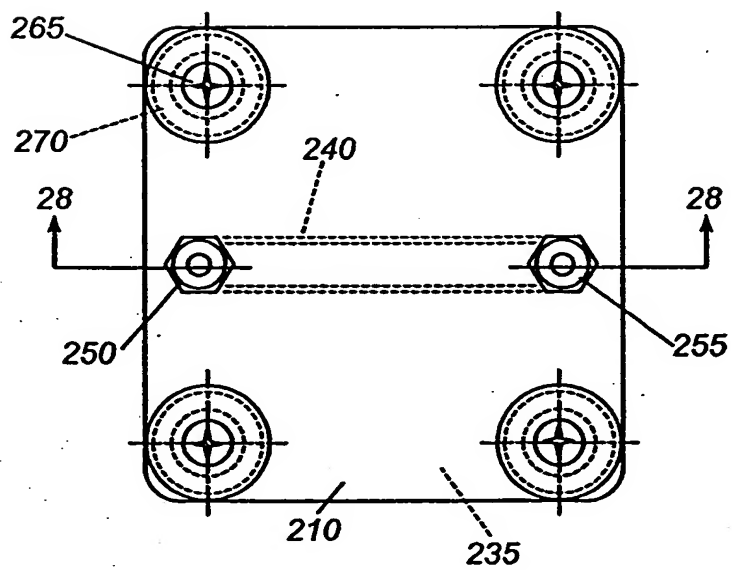
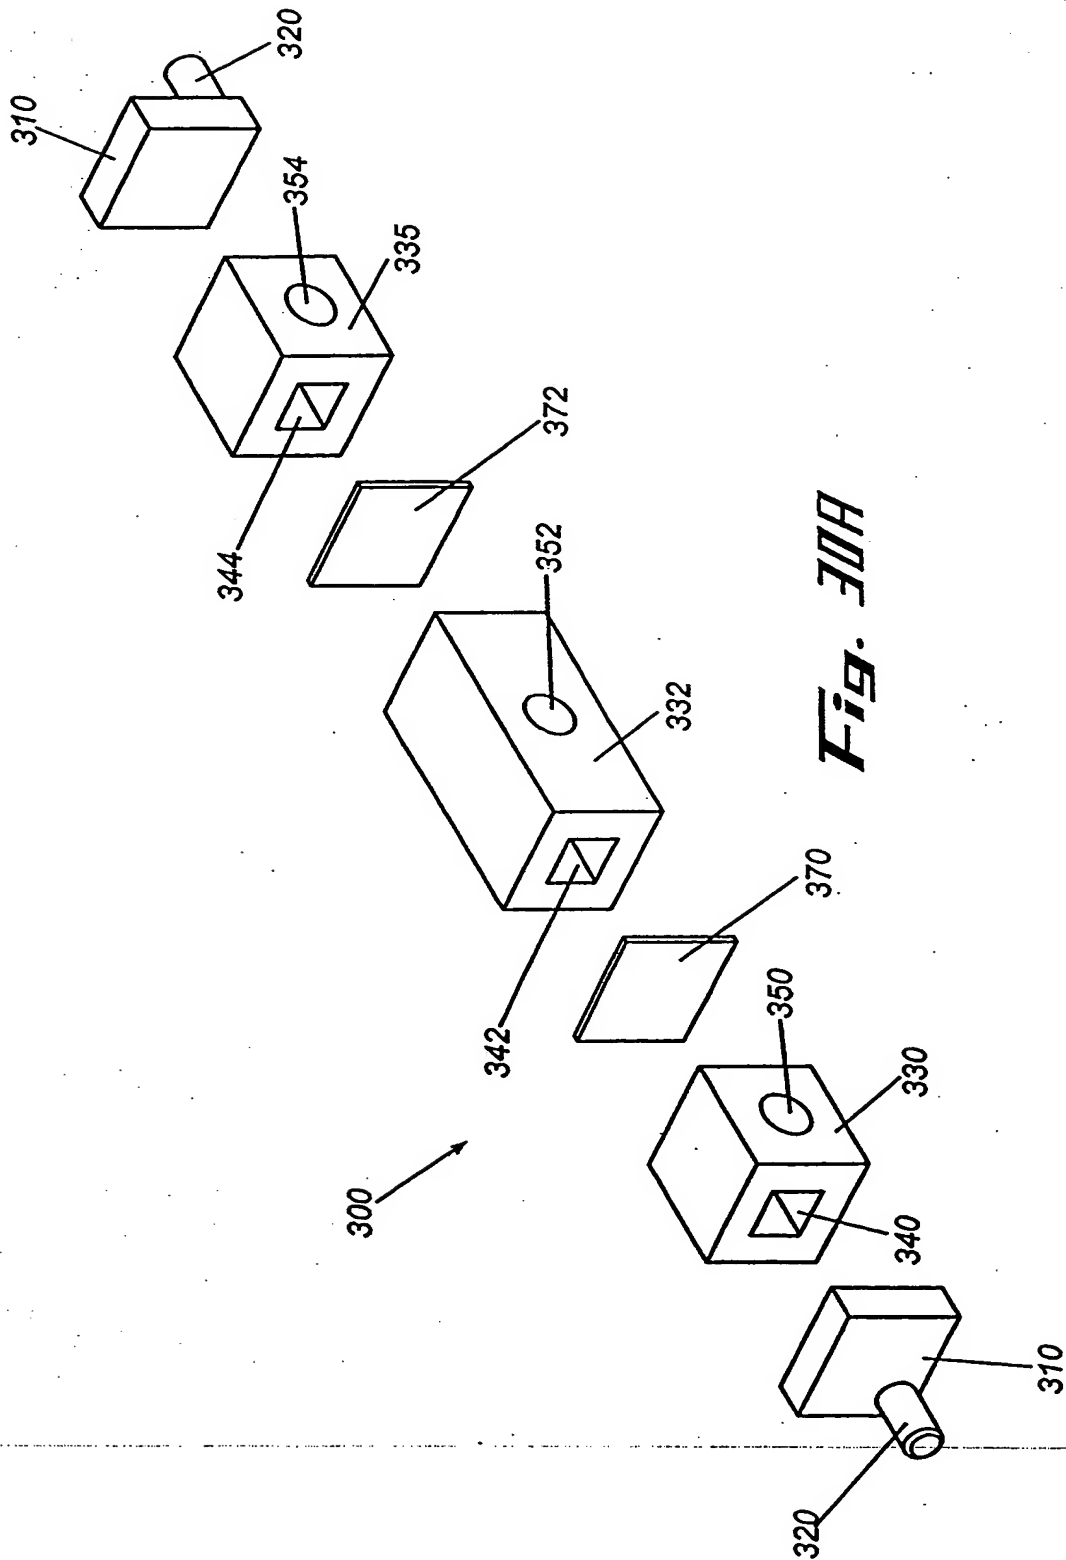


Fig. 29



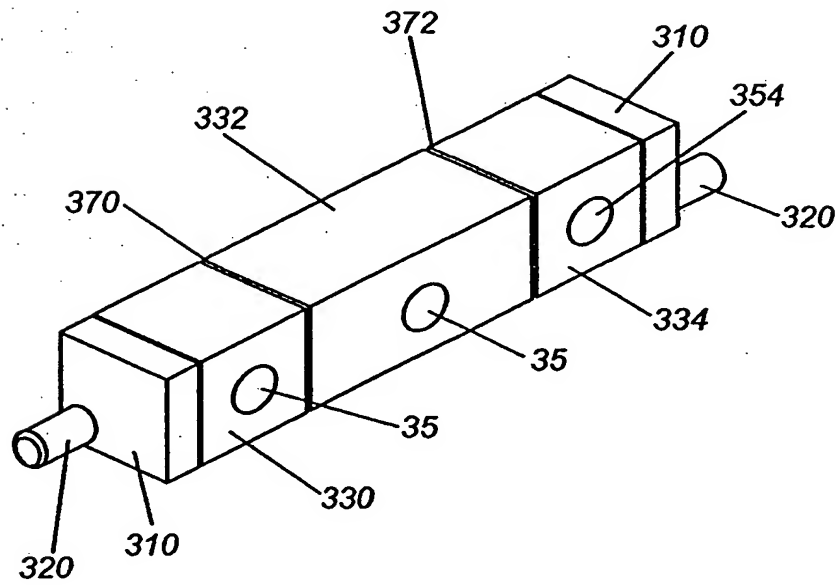


Fig. 30B

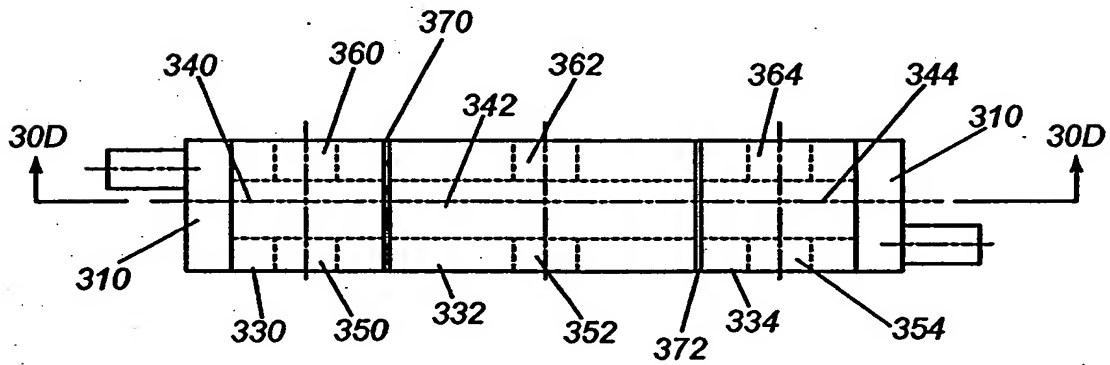


Fig. 30C

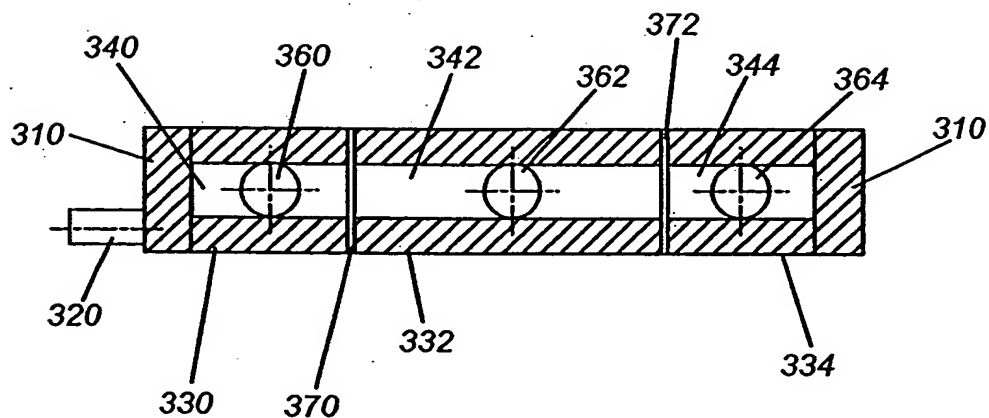


Fig. 30D




Fig. 30E


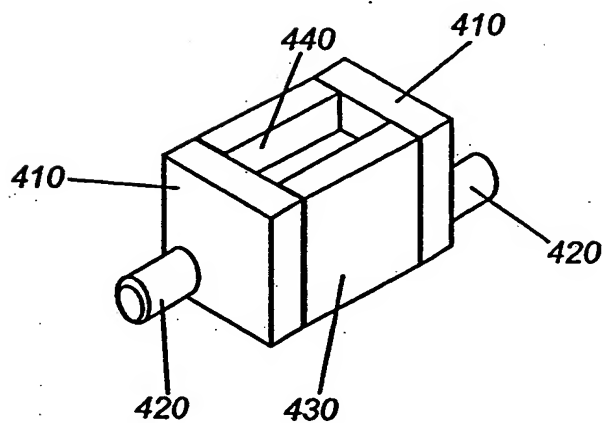
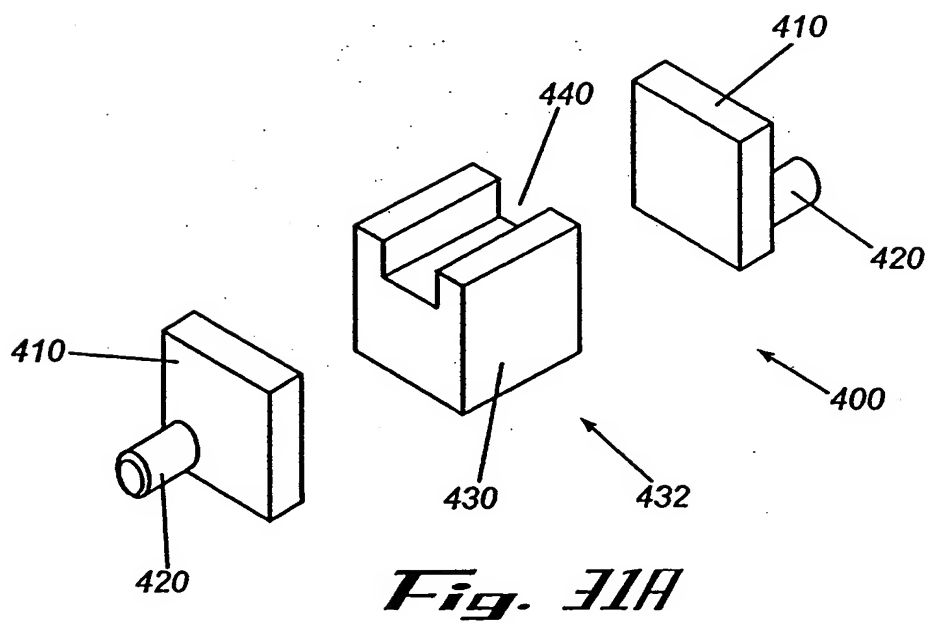


Fig. 30F



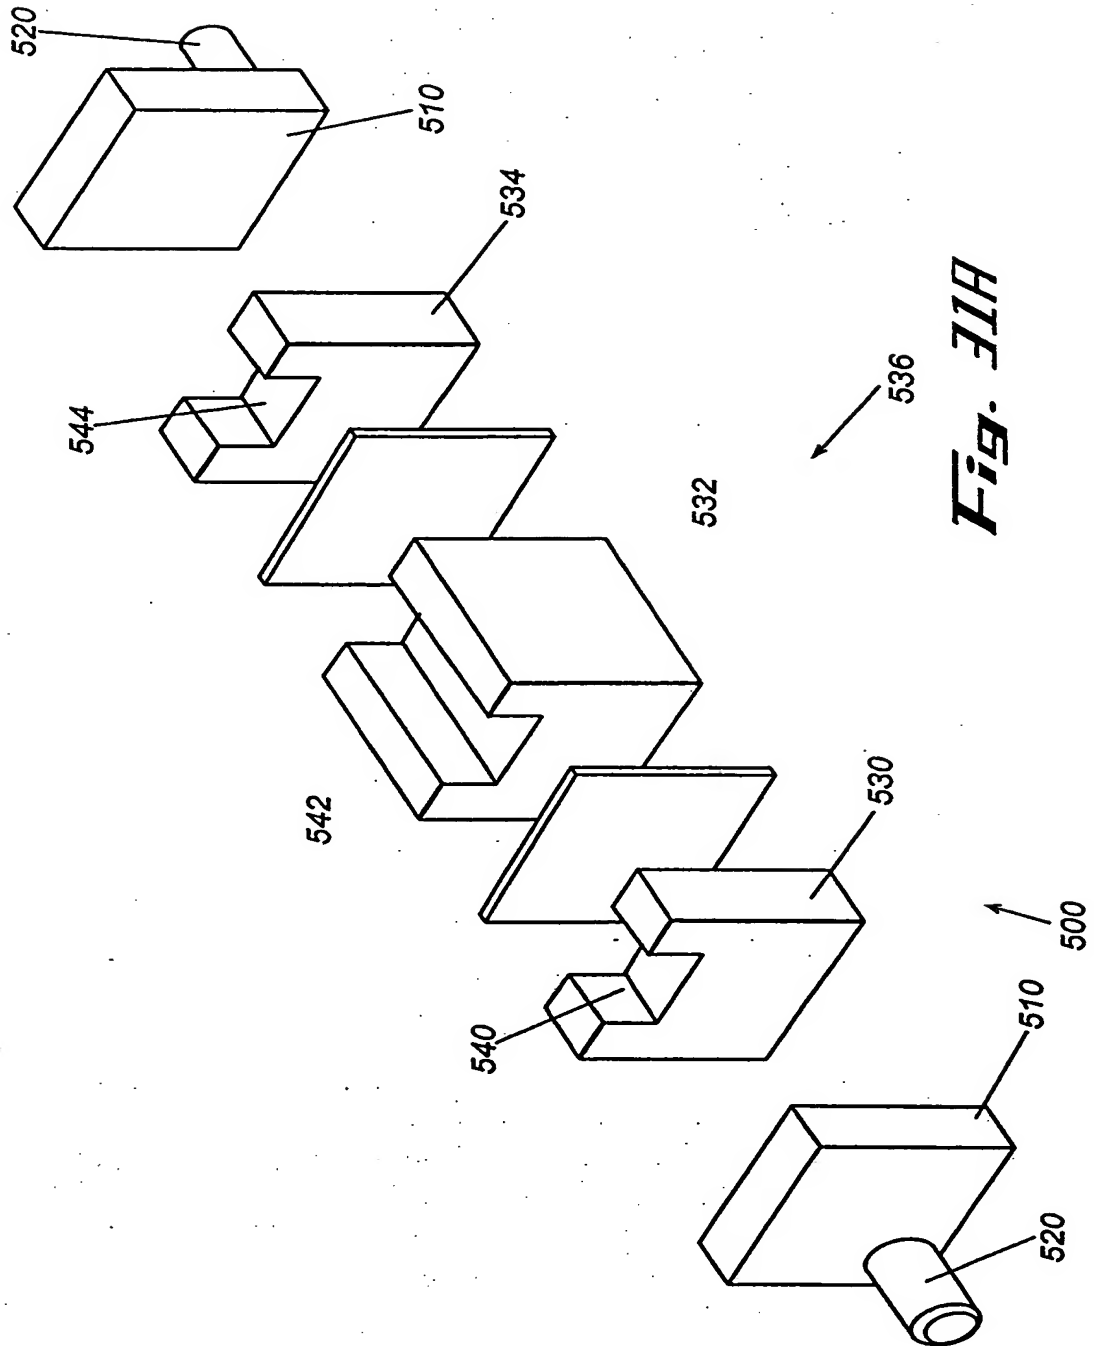


Fig. 31A

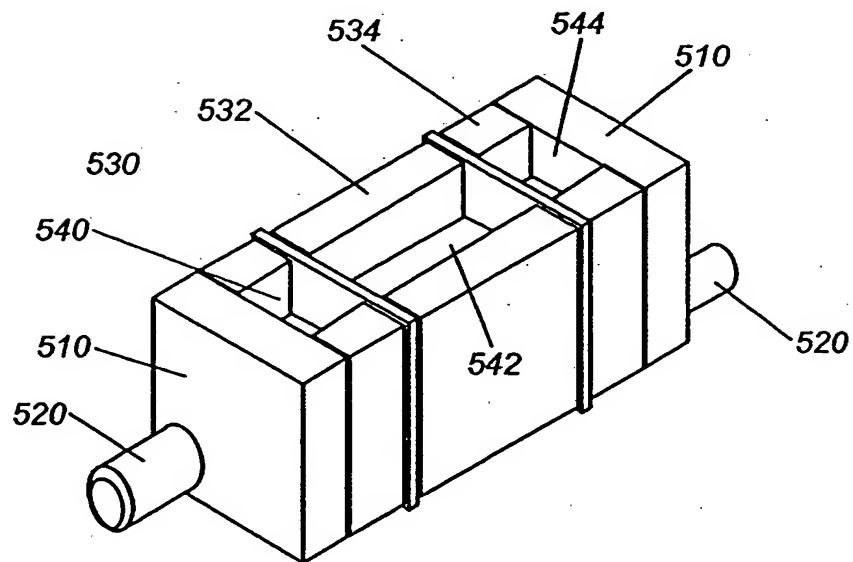


Fig. 32B

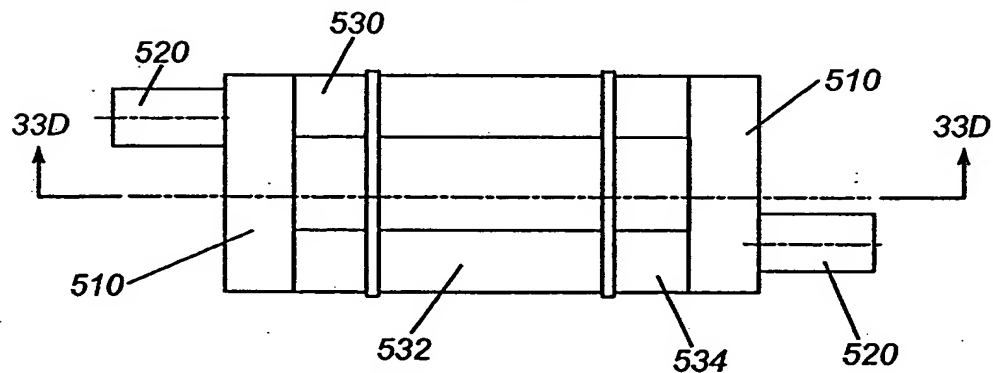


Fig. 32C

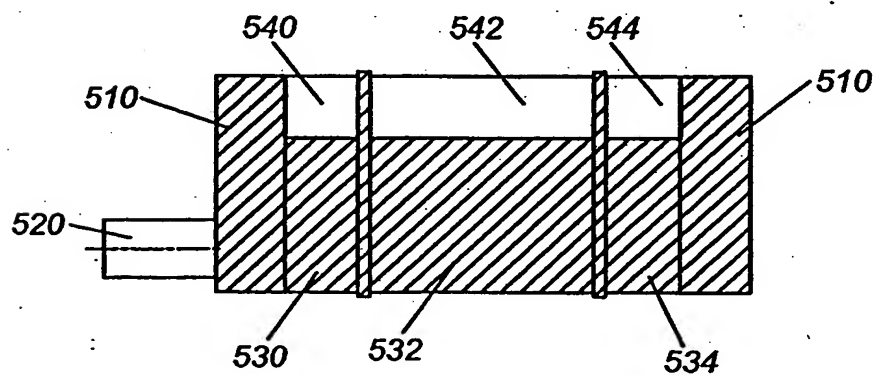


Fig. 32D

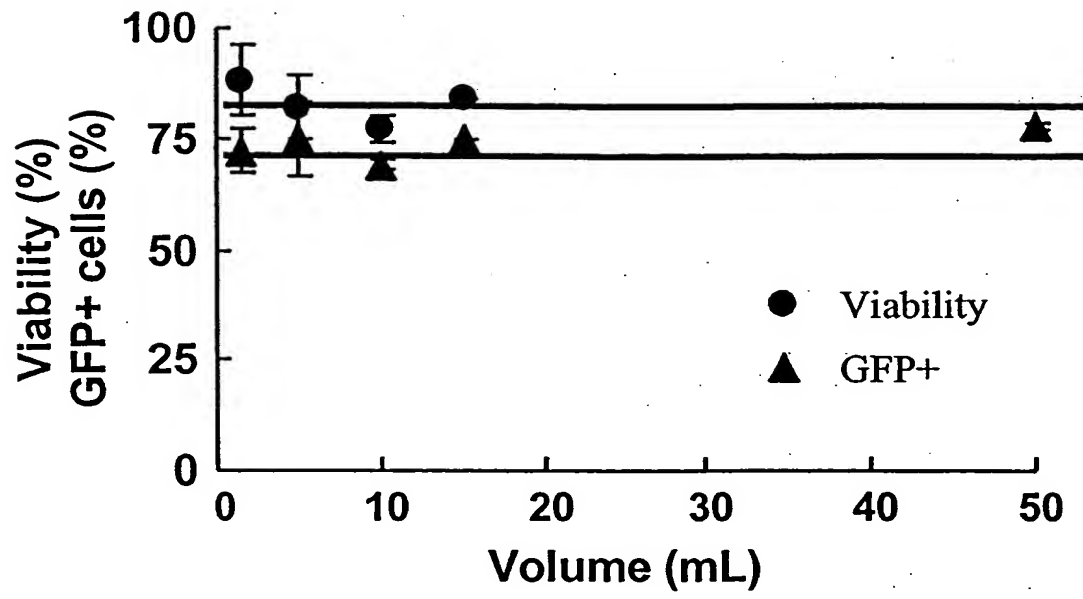


FIG. 33

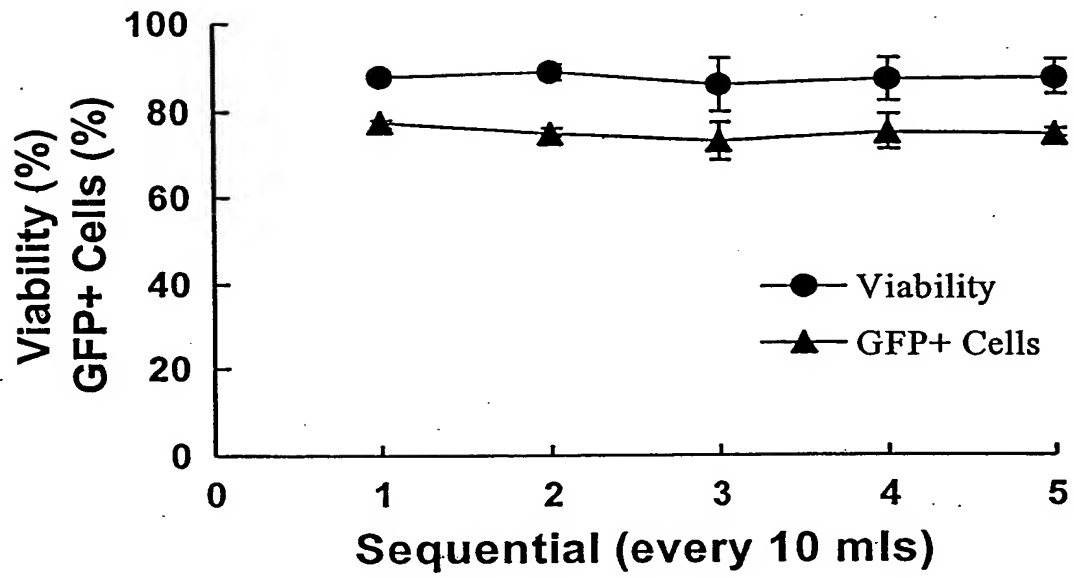


FIG. 34

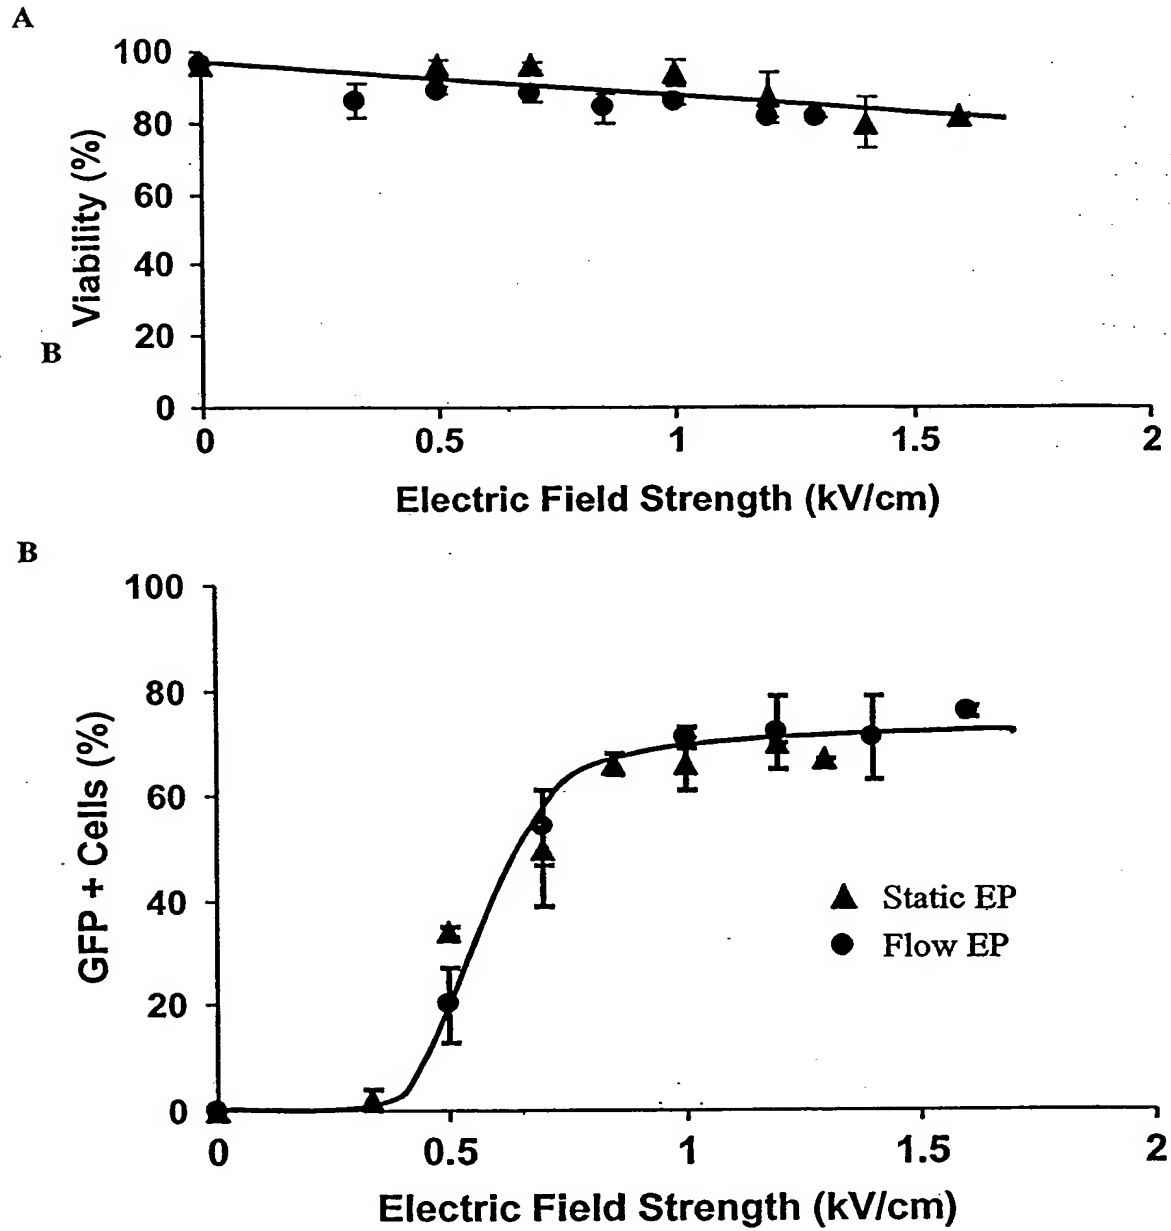


FIG. 35 and 36

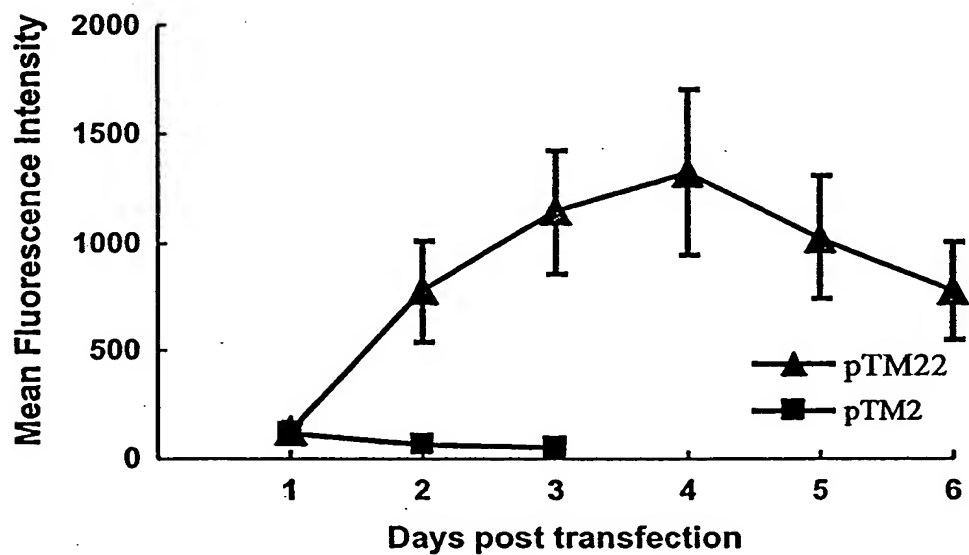
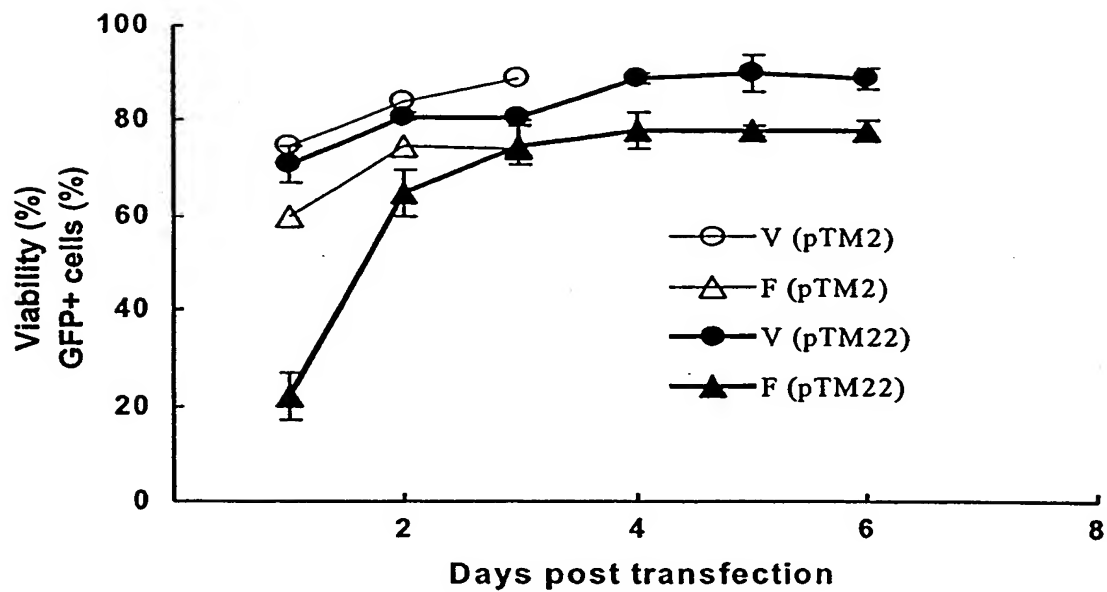


FIG. 37 and 38

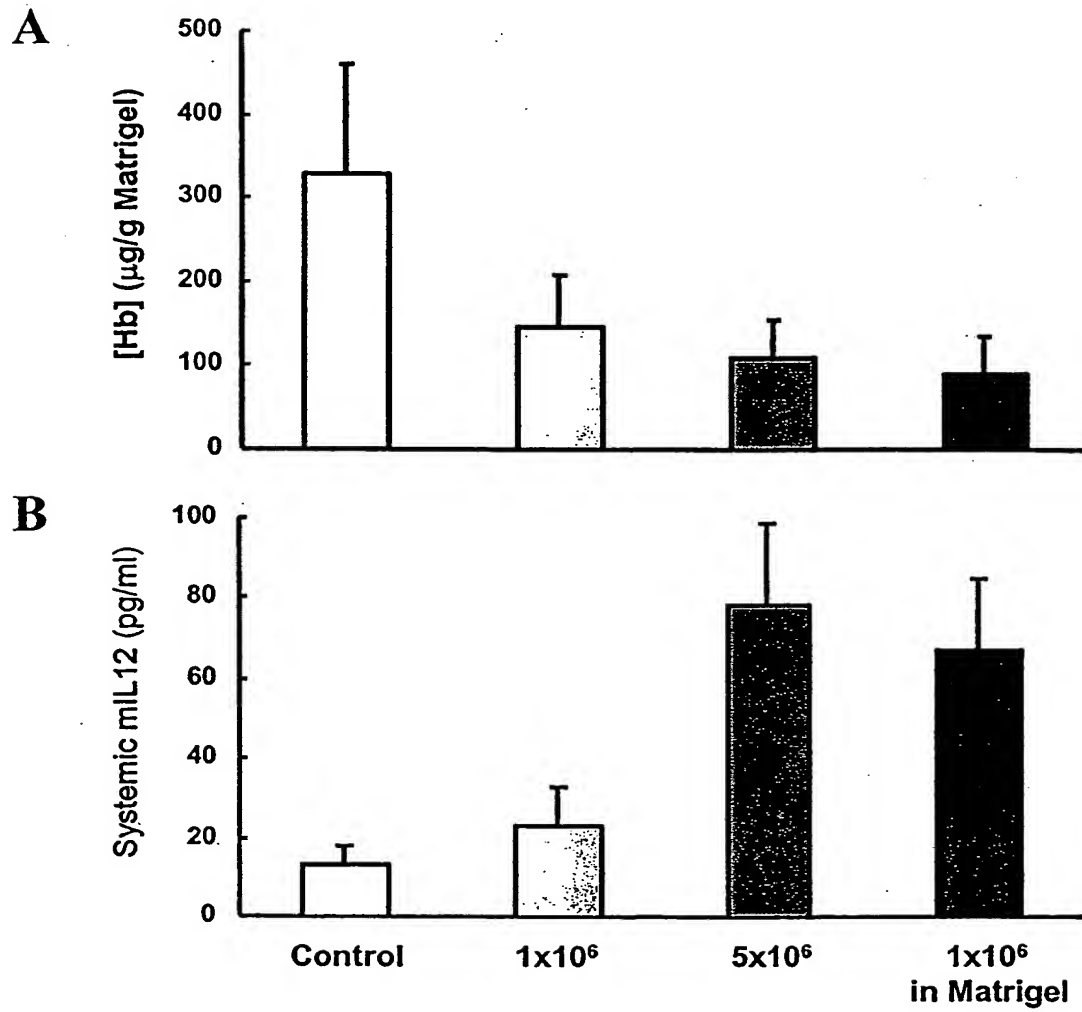


FIG. 39 and 40

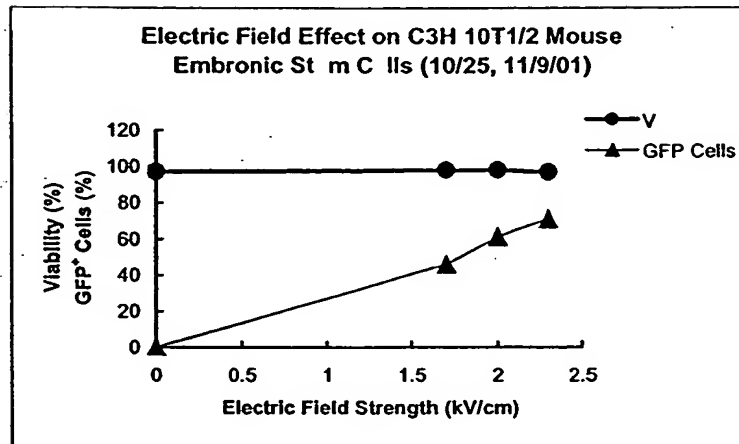


FIG. 41

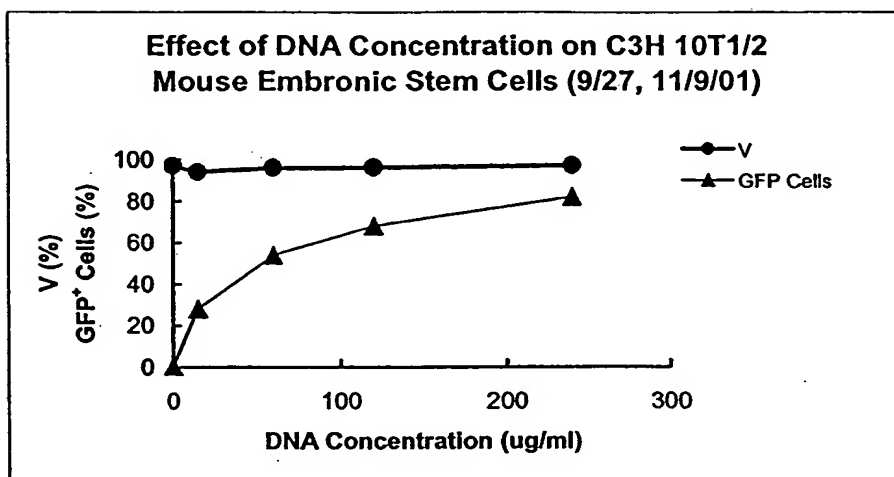


Fig. 42

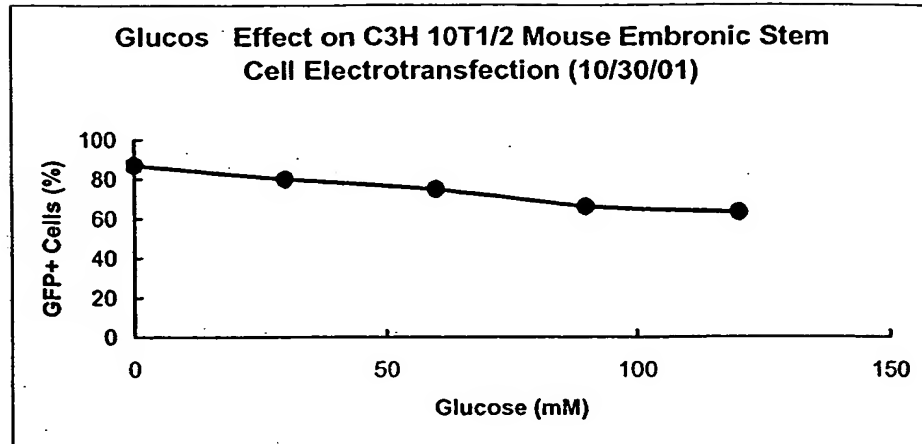


FIG. 43

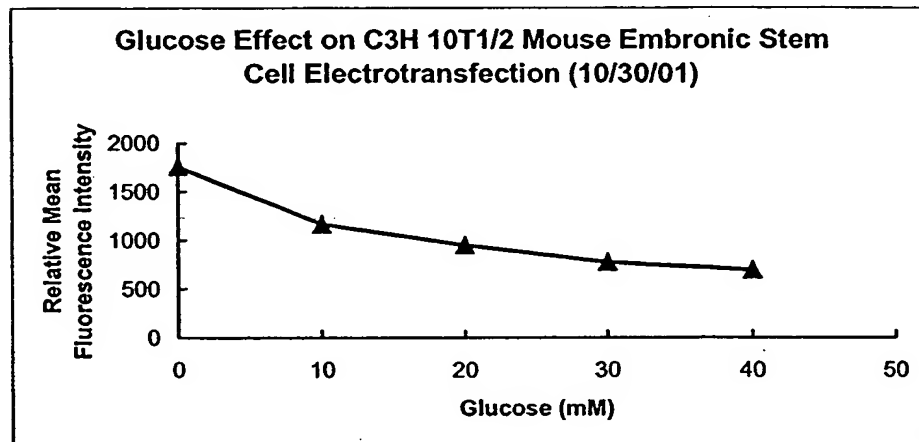


FIG. 44

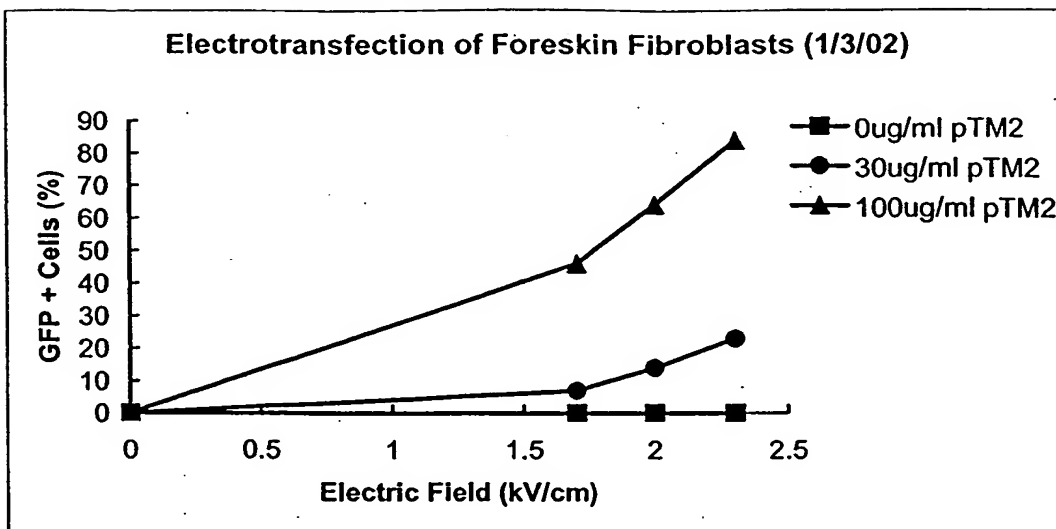


FIG. 45

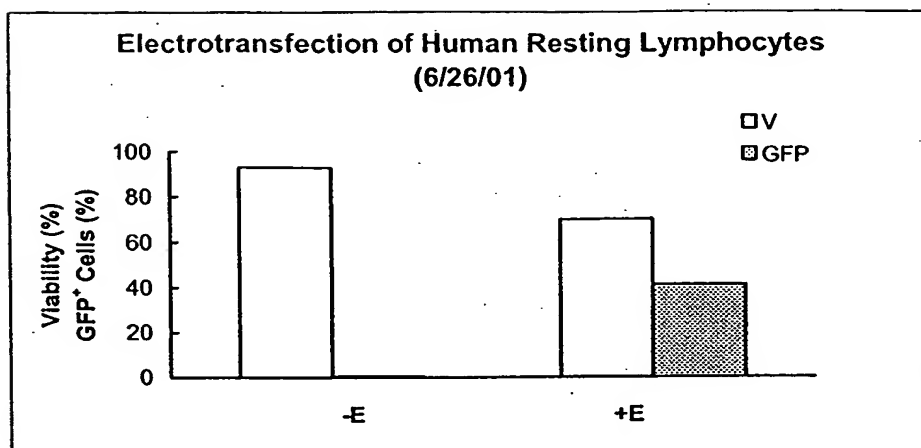


FIG. 46

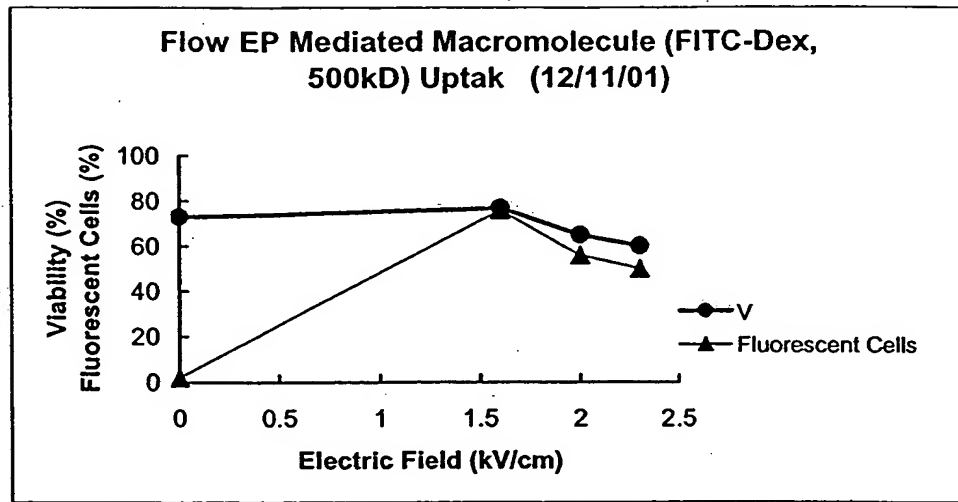


FIG. 47

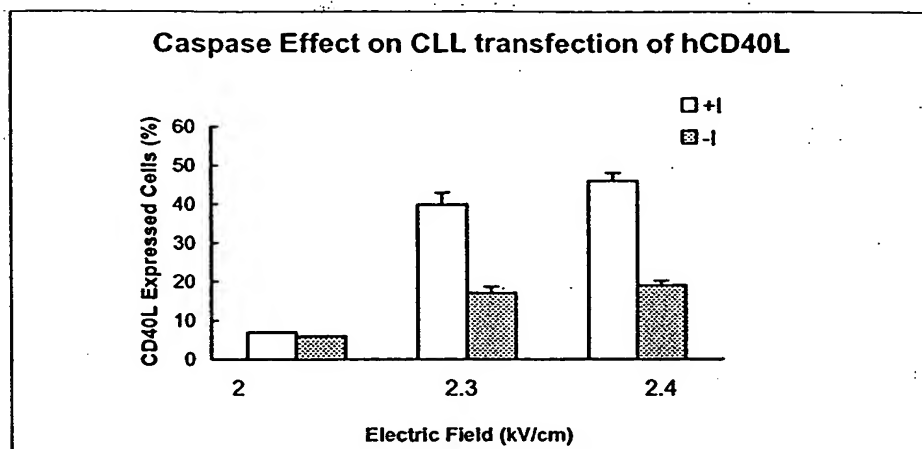


FIG. 48

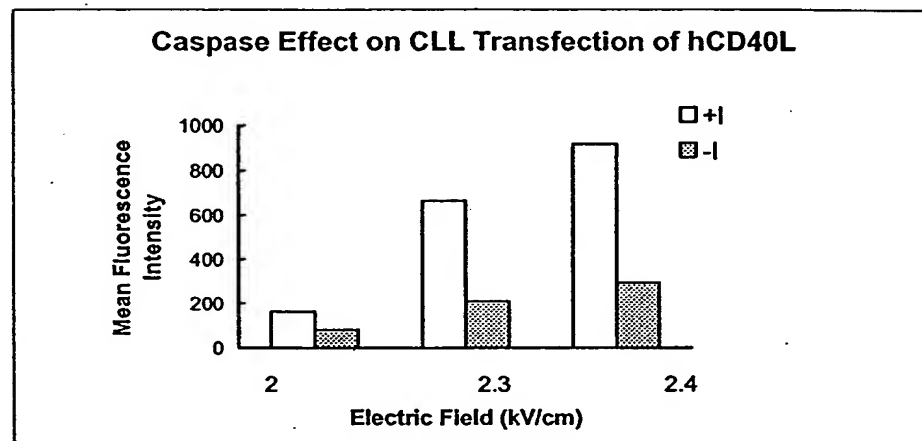


FIG. 49

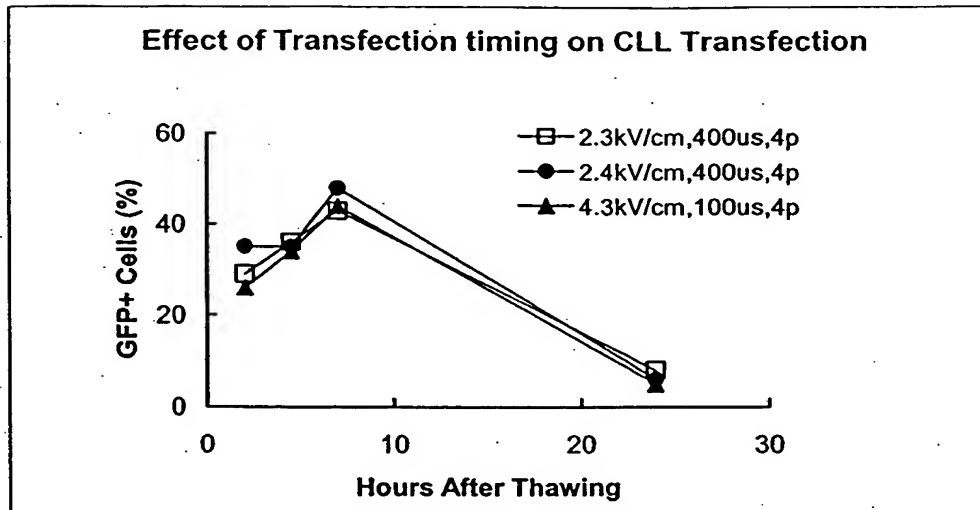


FIG. 50

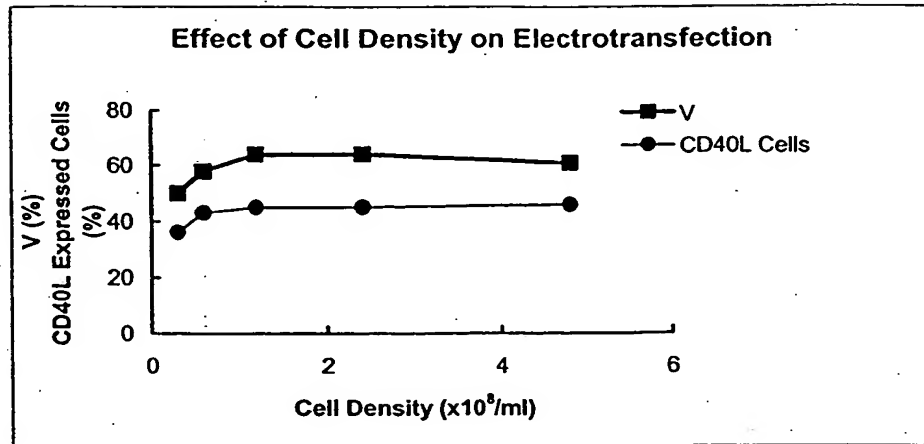


FIG. 51

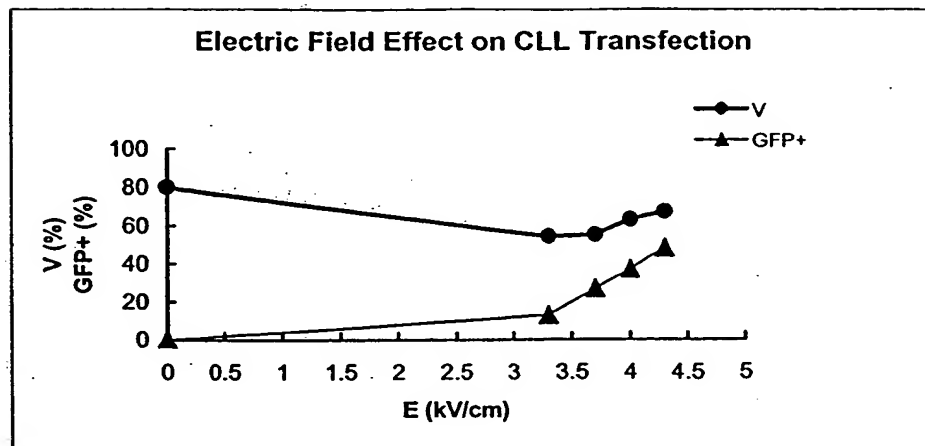


FIG. 52

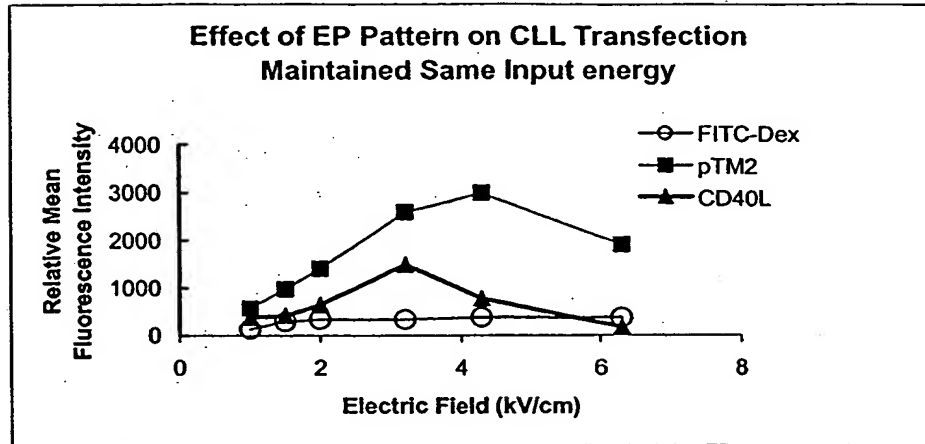


FIG. 53

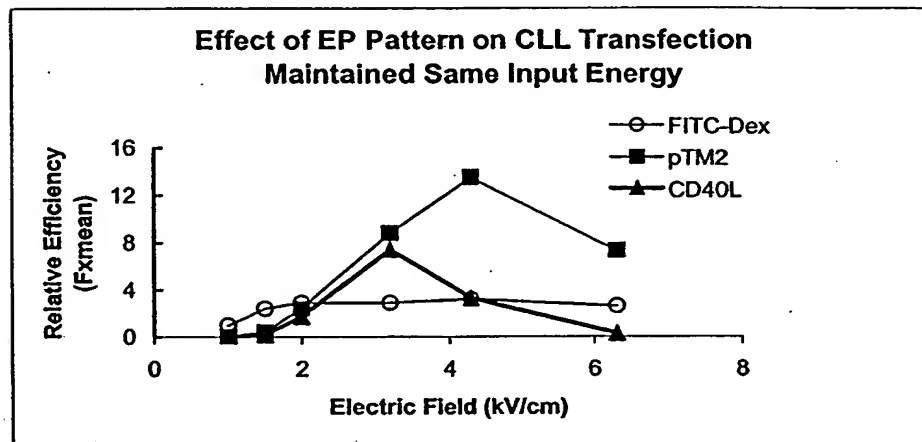


FIG. 54

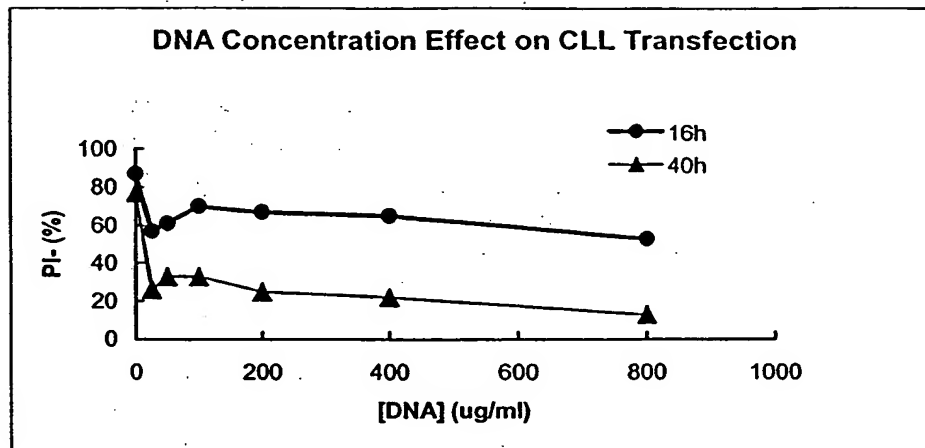


FIG. 55

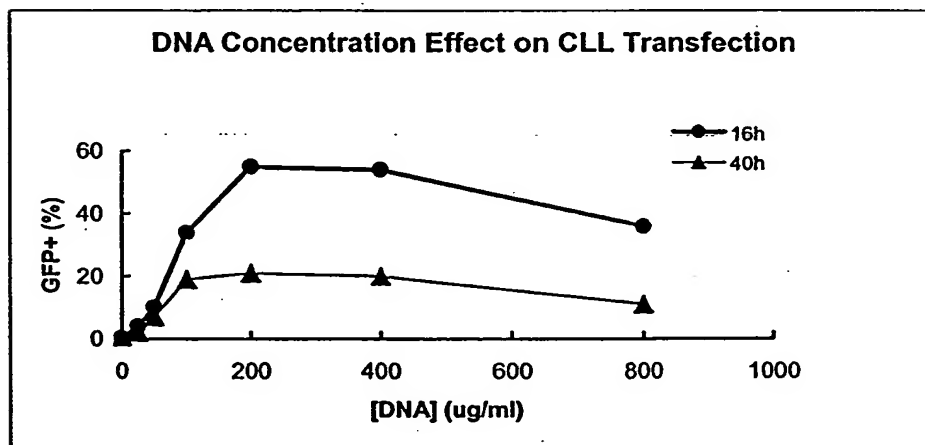


FIG. 56

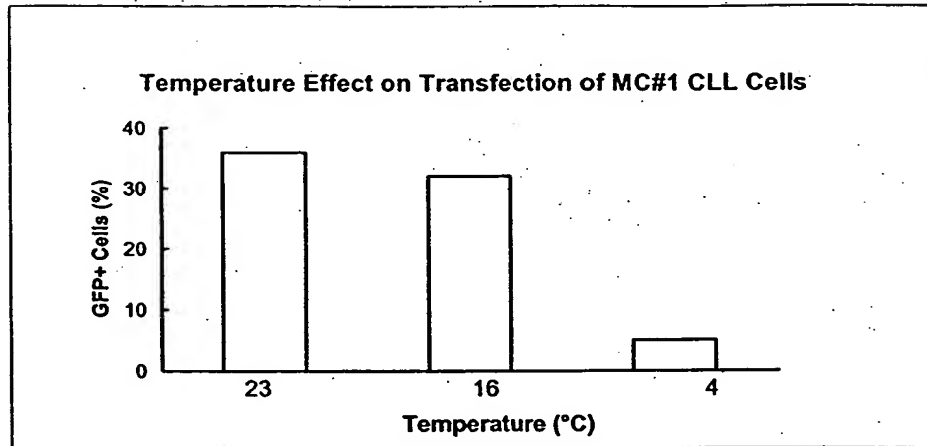


FIG. 57